




# TDCR: Triple-to-Double Coincidence Ratio

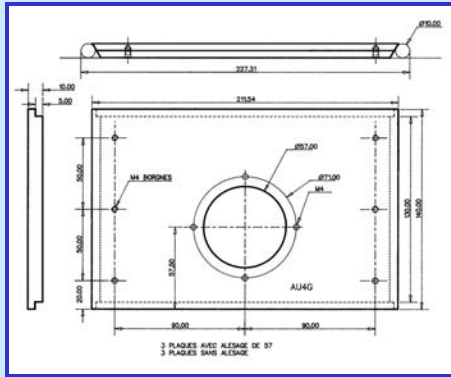


Side view of the measuring chamber

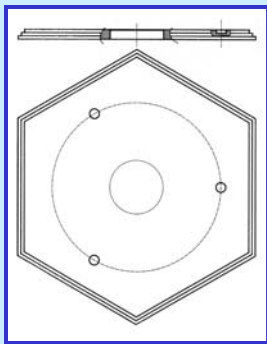


Cover of the measuring chamber

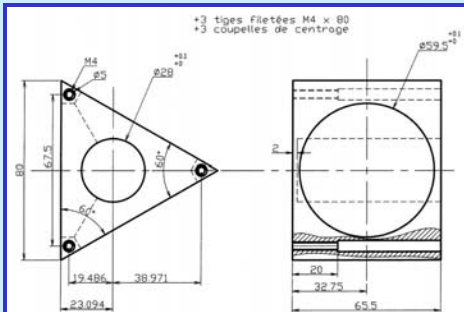


Source and photomultiplier holder

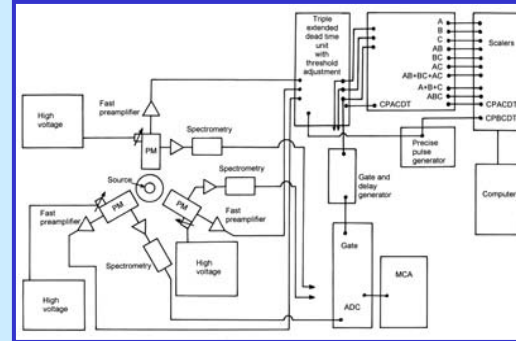

Schematic of experimental set up

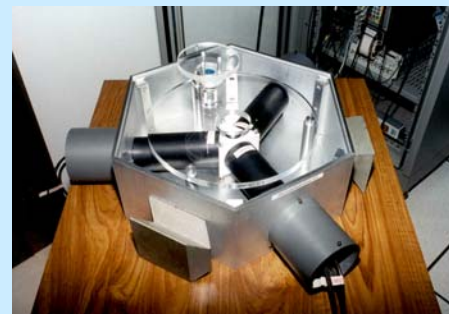


View of the counting set up

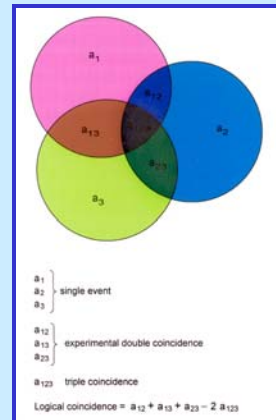

Logical relationship between different number of counts



Inner view of the coincidence unit

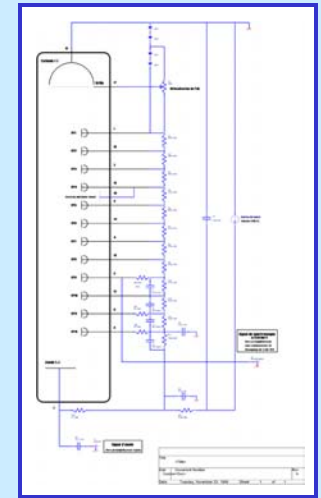

Schematic of a photomultiplier basis

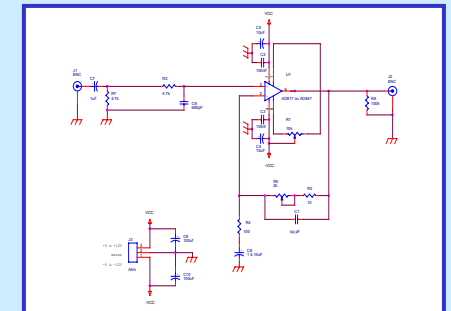


Diagram of a spectrometry preamplifier

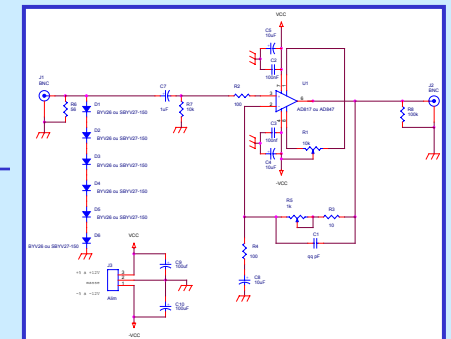


Diagram of an anode preamplifier