



**CIPM MRA**  
Comparison reports

---

# EURAMET.RI(I)-S19

---

## Air kerma in Am-241 and Co-60 radiation protection beams

**SUPPLEMENTARY COMPARISON**

© 2026, L. Persson *et al*

This report is published by the BIPM.

Original content from this Report may be used under the terms of the  
[Creative Commons Attribution 4.0 International \(CC BY 4.0\) Licence](https://creativecommons.org/licenses/by/4.0/).

---

Any further distribution of this Report must be cited as:  
L. Persson *et al* 2026 CIPM MRA Comparison reports 06003

<https://doi.org/10.59161/SZYA6566>

The CIPM MRA Comparison reports are made available under the Creative Commons Attribution International licence:

**Attribution 4.0 International (CC BY 4.0)**



By using this Report, you accept to be bound by the terms of this licence

(<https://creativecommons.org/licenses/by/4.0/>).

**Distribution** – you may distribute the Report according to the stipulations below.

**Attribution** – you must cite the Report.

**Adaptations** – you must cite the original Report, identify changes to the original and add the following text: This is an adaptation of an original Report by the Author(s). The opinions expressed and arguments employed in this adaptation should not be reported as representing the views of the Authors.

**Translations** – you must cite the original Report, identify changes to the original and add the following text: In the event of any discrepancy between the original work and the translation, only the text of the original Report should be considered valid.

**Third-party material** – the licence does not apply to third-party material in the Report. If using such material, you are responsible for obtaining permission from the third-party and of any claims of infringement.

# Supplementary comparison of air kerma standards in $^{60}\text{Co}$ and $^{241}\text{Am}$ radiation beams for radiation protection, EURAMET.RI(I)-S19

L.Persson<sup>1</sup>, EL Hansen<sup>2</sup>, PO Hetland<sup>2</sup>, N A Cornejo Díaz<sup>3</sup>, M Kelly<sup>4</sup>, J. Lillhök<sup>1</sup>, R. Nylund<sup>5</sup>, J. Huikari<sup>5</sup>

<sup>1</sup> Swedish Radiation Safety Authority, Stockholm Sweden

<sup>2</sup>Norwegian Radiation and Nuclear Safety Authority, Østerås, Norway

<sup>3</sup>Centre for Energy, Environment and Technology Research, Madrid, Spain

<sup>4</sup>National Physical Laboratory, Teddington, UK

<sup>5</sup>Radiation and Nuclear Safety Authority, Vantaa, Finland

## Abstract

A supplementary comparison of air kerma standards of five participating laboratories was carried out in  $^{241}\text{Am}$  and  $^{60}\text{Co}$  radiation beams at radiation protection level, from June 2024 to January 2025. Three of the participating laboratories are secondary standards laboratories (DSA, STUK, and SSM) and NPL and CIEMAT are primary standards laboratories, with NPL providing the reference values for the comparison. The comparison results are published in the BIPM key comparison database (KCDB) under the reference EURAMET.RI(I)-S19. The comparison was made indirectly using two ionization chambers as transfer instruments. The results are analysed and presented in terms of ratios of the calibration coefficients provided by the participants with respect to the comparison reference values.

## 1. Introduction

The National Metrology Laboratories for dosimetry quantities of Finland (STUK, Radiation and Nuclear Safety Authority), Norway (DSA, Norwegian Radiation and Nuclear Safety Authority), Spain (CIEMAT, Spanish National Metrology Institute for Ionising Radiation), Sweden (SSM, Swedish Radiation Safety Authority) and the United Kingdom of Great Britain and Northern Ireland (NPL, National Physical Laboratory) have performed a comparison in terms of air kerma in  $^{241}\text{Am}$  and  $^{60}\text{Co}$  radiation fields. NPL and CIEMAT are primary standards laboratories (PSDLs), with NPL providing the reference value. The other participating laboratories are secondary standards laboratories (SSDLs). STUK acted as the measuring pilot laboratory and SSM as the reporting pilot laboratory.

Three transfer chambers, two spherical Exradin A6 ionisation chambers and one PTW TN32003 (10 liter) chamber, were circulated among the participants, and each laboratory reported calibration coefficients and uncertainty budgets for those chambers in terms of air kerma. During the circulation of the chambers, the Exradin A6 XQ152602 chamber was found to be defective. The defect expressed itself as a high and unstable leakage (between 10 - 100 times normal leakage). Therefore, the results from XQ152602 have not been taken into consideration and the results are presented for the other two chambers.

The objective of the comparison is to support the ionising radiation CMCs of SSM, DSA, STUK, and CIEMAT in the dosimetry branch for the quantities of air kerma/rate from a  $^{241}\text{Am}$  and  $^{60}\text{Co}$  source at radiation protection levels. CIEMAT was not participating in the  $^{241}\text{Am}$  comparison.

The detailed technical protocol is available in the KCDB under the reference EURAMET.RI(I)-S19.

## 2. Comparison procedure

### 2.1 Participants and measurement schedule

Five participants, listed in table 1, were included in the  $^{60}\text{Co}$  comparison and four of them in the  $^{241}\text{Am}$  comparison. NPL provided the comparison reference values. STUK and SSM shared responsibilities as pilot laboratories: STUK acting as measuring pilot laboratory and SSM acting as the reporting laboratory. STUK performed measurements at the beginning, in the middle and at the end of the comparison to confirm the stability of the transfer chambers.

**Table 1.** Participants of the comparison, their traceability and the measurement schedule.

| Institute, country    | Contact person              | Comment               | Traceability, type of standard  | Measuring period      |
|-----------------------|-----------------------------|-----------------------|---|-----------------------|
| STUK                  | Jussi Huikari               | Pilot, measurements   | $^{60}\text{Co}$ PTB, secondary<br>$^{241}\text{Am}$ NPL, secondary                               | June-August 2024      |
| DSA                   | Per Otto Hetland            |                       | $^{60}\text{Co}$ IAEA, secondary<br>$^{241}\text{Am}$ VSL (via ISO N-80 X-ray quality), secondary | August-September 2024 |
| NPL                   | Martin Kelly                | Reference value       | NPL, primary  | October 2024          |
| STUK, stability check |                             |                       |   | October 2024          |
| SSM                   | Linda Persson               | Pilot, reporting      | $^{60}\text{Co}$ BIPM, secondary<br>$^{241}\text{Am}$ NPL, secondary                              | October 2024          |
| CIEMAT                | Néstor Armando Cornejo Díaz | Only $^{60}\text{Co}$ | CIEMAT, primary   | December 2024         |
| STUK, stability check |                             |                       |   | 13-17 January 2025    |

### 2.2 Transfer instruments

Two reference ionisation chambers, Exradin A6 and PTW TN32003, were used as transfer instruments for this comparison. The Exradin A6 chamber is the property of STUK and the PTW TN32003 chamber is the property of SSM, and they had not been calibrated outside STUK and SSM before this comparison. The laboratories used their own electrometers and cables for performing the measurements during the comparison. The technical details of the transfer chambers are presented below (table 2).

**Table 2.** Technical details of the transfer chambers

| Chamber type                                      | EXRADIN A6<br>Ref. 92716   | PTW TN32003  |
|---|--|--|
| Serial number                                     | XQ200282   | 000296   |
| Geometry  | spherical  | spherical  |
| Wall material                                     | C552   | POM (polyoxymethylene)   |
| Wall thickness<br>[mm]                            | 3.0  | 3.0  |
| External diameter / mm                            | 120  | 276  |
| Nominal volume / cm <sup>3</sup>                  | 800  | 10000  |
| Reference point for the<br>air kerma measurements | Geometric centre of the chamber  | Geometric centre of the chamber  |
| Polarising voltage of the<br>chamber              | +400 V on collector (central)<br>electrode, 0 V on chamber wall<br>(collecting negative charge)<br>(if +400 V on collector is not<br>available: -400 V on chamber<br>wall, 0 V on collector electrode) | +400 V on collector (central)<br>electrode, 0 V on chamber wall<br>(collecting negative charge)<br>(if +400 V on collector is not<br>available: -400 V on chamber<br>wall, 0 V on collector electrode) |
| Connector type                                    | Triax BNC (male) (2 lug)   | Triax BNC (male) (2 lug)   |

## 2.3 Radiation quality and reference conditions

The radiation qualities used in the comparison are <sup>241</sup>Am and <sup>60</sup>Co at radiation protection level. The quantity used for the comparison is the air kerma defined according to ICRU85a. The relevant data from ICRU90 has been used for the primary standards from participants in the comparison and for primary standards against which the secondary standards have been calibrated.

The radiation protection level radiation fields for <sup>241</sup>Am and <sup>60</sup>Co fulfil the standards ISO 4037-1:2019 (Annex B in case of <sup>241</sup>Am) and ISO 4037-2:2019. The reference point for the chambers is the geometric centre of the chambers. The chambers were placed free in air with the marking on the stem oriented towards the radiation source. The diameter of the radiation fields can for each participant be found in Appendix 1.

The calibration coefficients for the transfer chambers are corrected to standard conditions of air temperature and pressure;  $T = 293.15$  K and  $P = 101.325$  kPa. The measurements were performed with relative humidity between 38 % and 70 %; therefore, they were not corrected to the reference condition of 50 % RH. Each laboratory was using its own equipment to measure environmental conditions and ensuring traceability for those measurements.

## 2.4 Reference value

NPL provided the reference values for this comparison as a primary standards laboratory with all relevant CMC entries. All results were compared to these values. STUK and SSM are traceable to NPL for the <sup>241</sup>Am air kerma. None of the four laboratories is traceable to NPL for <sup>60</sup>Co air kerma.

Realization of the quantity is performed at NPL using their air kerma standards, based on graphite-walled cavity ionisation chambers as described in the respective reports (Bass GA. *et al.* 2019a and Bass GA. *et al.* 2019b).

For <sup>60</sup>Co at protection level, CIEMAT has recently implemented its own traceability based on the primary standard for <sup>137</sup>Cs (Cornejo, 2022 and Kessler C. *et al.*, 2024) and the use of a beam

quality correction factor ( $k_{Co,Cs}$ ) for a well-characterized secondary standard ionization chamber (Cornejo Díaz *et al.* 2024).

For determining calibration coefficients for the transfer chambers, NPL and CIEMAT proceeded as the other laboratories according to section 2.5 excluding the procedure for determining the reference air kerma/ air kerma rate.

## 2.5 Determination of the calibration coefficient of the transfer chamber

Each laboratory used their own procedure referring to international practices/guidance followed when performing the calibration.

Typically, for air kerma, the SSDLs establish a reference air kerma rate  $\dot{K}_{air,lab}$  at their facilities in accordance with their own procedure following an equation such as:

$$\dot{K}_{air,lab} = N_{K,PSDL} \cdot I_{lab} \quad (1)$$

where  $N_{K,PSDL}$  is the calibration coefficient of the secondary standard used by a given laboratory in order to establish traceability to a primary standards laboratory for air kerma in  $^{241}\text{Am}$  or  $^{60}\text{Co}$  beams, and where  $I_{lab}$  is the ionisation current measured by the participant with the secondary standard at the reference calibration point.  $I_{lab}$  is corrected to standard conditions of air temperature and pressure, and, if needed, for relative humidity. For the other corrections to  $I_{lab}$  each laboratory proceeded according to their own procedure and may have included e.g. the electrometer correction factor, correction for leakage, correction for distance, correction for volume etc. All corrections used by the participants are reported in Appendix 1.

Each laboratory positioned the transfer chambers (see table 2) at the reference point, and the calibration coefficient for each transfer chamber,  $N_K$ , was calculated as:

$$N_{K,lab} = \frac{\dot{K}_{air,lab}}{I_{M,lab}} \quad (2)$$

where  $\dot{K}_{air,lab}$  is the reference air kerma rate from equation (1), and  $I_{M,lab}$  is the ionization current measured by the laboratory with the transfer chamber. Like  $I_{lab}$ ,  $I_{M,lab}$  was corrected to standard conditions of air temperature and atmospheric pressure. The correction for the air relative humidity was not required, according to Section 2.3.

## 2.6 Ratios of the calibration coefficients

The ratios of the calibration coefficients are evaluated as follows for each participating laboratory, separately for each transfer chamber and beam quality:

$$R_{lab} = \frac{N_{K,lab}}{N_{K,NPL}} \quad (3)$$

where  $N_{K,lab}$  is the calibration coefficient reported by the participating laboratory for a given transfer chamber and radiation quality, and  $N_{K,NPL}$  is the corresponding calibration coefficient provided by the NPL and adopted as reference in this comparison.

There were two transfer chambers, and for each of the two radiation qualities, the laboratory ratio of the calibration coefficients was calculated as the average of the ratios obtained with each of the transfer chambers:

$$R_{lab} = \frac{1}{2} \sum_{i=1}^2 \frac{N_{K,lab,i}}{N_{K,NPL,i}} \quad (4)$$

where  $N_{K,lab,i}$  and  $N_{K,NPL,i}$  are the calibration coefficients provided by the participating laboratory and the NPL, respectively, for transfer chamber  $i$ .

The variance of  $R_{lab}$ , denoted as  $u_{R,lab}^2$ , is calculated as the average of the variances of the calibration coefficient ratios obtained for each transfer chamber  $i$ , ( $u_{R,lab,i}^2$ ):

$$u_{R,lab,i}^2 = (u_{lab}^2 + u_{NPL}^2 - \sum_j f_j^2 (u_{lab,j}^2))_i + u_{tr,i}^2 \quad (5)$$

where  $u_{lab}$  is the combined standard uncertainty of the calibration coefficient reported by the participating laboratory;  $u_{NPL}$  is the combined standard uncertainty of the NPL's calibration coefficient ( $N_{K,NPL}$ );  $u_{tr}$  is the uncertainty arising from the transfer chamber stability and  $f_j$  are the correlation factors related to the uncertainty components  $j$  that are correlated between the participating laboratory and the NPL. The physical constants involved in air kerma determinations by the primary standards laboratories have been considered to be fully correlated ( $f_j = 1$ ), as well as all of the non-statistical components of  $u_{NPL}$  for those participating laboratories traceable to the NPL.

In equation (5),  $u_{tr}$  combines the stability of the transfer chambers over the period of the comparison. The measuring pilot laboratory STUK has performed several measurements for the transfer chamber.

The expanded uncertainty of  $R_{lab}$  is calculated as:  $U_{lab} = 2 u_{R,lab}$ .

## 2.7 Correlated uncertainties for comparison ratios

Correlated uncertainties were analysed and excluded from the calculation of expanded uncertainties of the ratios of calibration coefficients. STUK and SSM are directly traceable to NPL for  $^{241}\text{Am}$  air kerma. The component of the NPL calibration related to the primary standard measurement was removed in all cases where the laboratory is traceable to NPL, i.e. STUK and SSM for  $^{241}\text{Am}$  air kerma. For all other cases, the correlated components related to the physical constants were removed.

## 3. Results

### 3.1 Transfer chamber stability and recombination

The transfer chambers were calibrated in terms of air kerma in  $^{241}\text{Am}$  and  $^{60}\text{Co}$  beams by STUK at the beginning, in the middle and at the end of the measurement round. In total, there were 7 (for  $^{241}\text{Am}$ ) and 10 (for  $^{60}\text{Co}$ ) stability check measurements for each of the transfer chambers. The standard uncertainty of the mean value for the transfer chamber,  $u_{tr}$ , was found to be 0.033% for the Exradin chamber and 0.075% for the PTW chamber, which shows that the chambers were stable during the measurement round.

The pilot laboratory did not apply corrections for lack of saturation of the circulated transfer chambers, using the information provided by the participating laboratories. The corrections for

lack of saturation are expected to be more significant for the PTW 32003 chamber with 10000 cm<sup>3</sup> collecting volume than for the Exradin A6 chamber (800 cm<sup>3</sup>) considering the actual air kerma rates (both chambers are spherical and operated with the same polarizing voltage). For the PTW 32003 chamber, the nominal air kerma rate for a 99 % saturation current is 26 mGy/h, according to the user manual provided by the manufacturer. This value is significantly higher than the maximum value reported by the participants. Furthermore, taking into account previous studies done with the CIEMAT secondary standard ionisation chambers, the corrections for lack of saturation in case of the PTW 32003 chamber varied between 1.0019 and 1.0020 for <sup>241</sup>Am and between 1.0019 and 1.0032 for <sup>60</sup>Co, with an uncertainty of 0.09 % ( $k = 1$ ). The impact of the variation of these corrections, due to the volumetric component of the ion recombination (as consequence of air kerma rate variations between laboratories) would be negligible for <sup>241</sup>Am and about 0.15 % (maximum variation) in the case of <sup>60</sup>Co. An uncertainty component to account for this non-corrected effect was included in the CIEMAT, NPL and SSM uncertainty budgets, for the transfer chambers. STUK and DSA consider the effect negligible.

### 3.2 Calibration coefficients and uncertainties

The calibration coefficients reported by the participating laboratories and their uncertainties are given in table 3 and 4 below. Detailed uncertainty budgets for each laboratory are given in Appendix 1.

**Table 3.** Reported calibration coefficients (Gy/C) for transfer chambers in terms of air kerma and their respective relative expanded uncertainties,  $U$ , (%), for <sup>241</sup>Am radiation quality.

| Institute | EXRADIN A6, Ref. 92716,<br>serial number XQ200282 |                | PTW TN32003, serial number<br>000296 |                |
|-----------|---|----------------|--------------------------------------|----------------|
|           | $N_{K,lab}$ (Gy/C)                                | $U(\%), k = 2$ | $N_{K,lab}$ (Gy/C)                   | $U(\%), k = 2$ |
| STUK      | 36820   | 4.33           | 3020                                 | 4.33           |
| DSA       | 36527   | 1.74           | 3008                                 | 1.89           |
| NPL       | 36880   | 2.04           | 3035                                 | 2.04           |
| SSM       | 36870   | 2.10           | 3042                                 | 2.20           |

**Table 4.** Reported calibration coefficients (Gy/C) for transfer chambers in terms of air kerma and their respective relative expanded uncertainties,  $U$ , (%), for <sup>60</sup>Co radiation quality.

| Institute | EXRADIN A6, Ref. 92716,<br>serial number XQ200282 |                | PTW TN32003, serial number<br>000296 |                |
|-----------|---|----------------|--------------------------------------|----------------|
|           | $N_{K,lab}$ (Gy/C)                                | $U(\%), k = 2$ | $N_{K,lab}$ (Gy/C)                   | $U(\%), k = 2$ |
| STUK      | 36915   | 1.09           | 3025                                 | 1.09           |
| DSA       | 36627   | 1.94           | 3012                                 | 2.33           |
| NPL       | 36980   | 1.46           | 3032                                 | 1.46           |
| SSM       | 36910   | 1.30           | 3030                                 | 1.40           |
| CIEMAT    | 36785   | 1.40           | 3004                                 | 1.47           |


### 3.3 Final results of the comparison

The ratios of the calibration coefficients ( $R_{lab}$ ) and their expanded uncertainties ( $U_{lab}$ ,  $k = 2$ ) were calculated according to equations 3-5. The following tables and figures (tables 5 and figure 1; and table 6 and figure 2), summarize the values of  $R_{lab}$  and  $U_{lab}$  obtained in this comparison by the participating laboratories for both radiation qualities.

**Table 5.** Ratios of calibration coefficients ( $R_{lab}$ ) and their expanded uncertainties ( $U_{lab}$ ) for participating laboratories in terms of air kerma for  $^{241}\text{Am}$  radiation quality.

| <b>Institute</b> | <b><math>R_{lab}</math></b> | <b><math>U_{lab}, k = 2</math></b> |
|------------------|-----------------------------|------------------------------------|
| STUK             | 0.997                       | 0.047                              |
| DSA              | 0.991                       | 0.028                              |
| NPL*             | 1.000                       | 0.020                              |
| SSM              | 1.001                       | 0.028                              |

\*for NPL, as providing the reference value, the expanded uncertainty is the reported uncertainty from NPL.

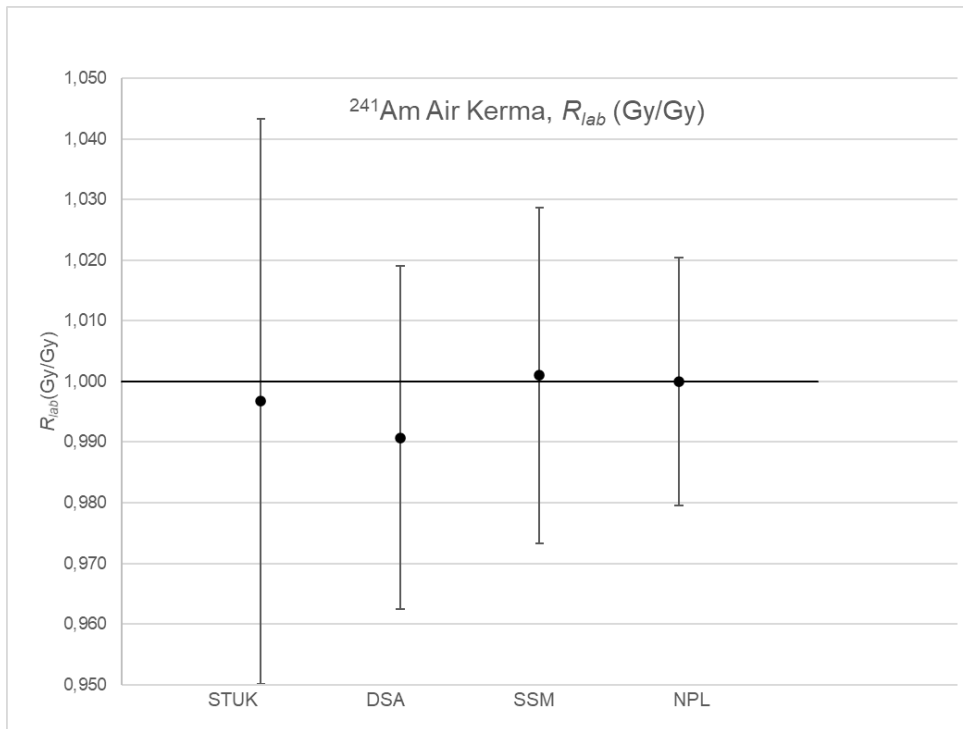


**Figure 1.** Graphical representation of the results in table 5: Ratios of calibration coefficients ( $R_{lab}$ ) and their expanded uncertainties ( $U_{lab}, k = 2$ ) for participating laboratories in terms of air kerma for <sup>241</sup>Am radiation quality.

**Table 6.** Ratios of calibration coefficients ( $R_{lab}$ ) and their expanded uncertainties ( $U_{lab}$ ) for participating laboratories in terms of air kerma for <sup>60</sup>Co radiation quality.

| Institute | $R_{lab}$ | $U_{lab}, k = 2$ |
|-----------|-----------|------------------|
| STUK      | 0.998     | 0.018            |
| DSA       | 0.992     | 0.026            |
| NPL*      | 1.000     | 0.015            |
| SSM       | 0.999     | 0.020            |
| CIEMAT    | 0.993     | 0.020            |

\*for NPL, as providing the reference value, the expanded uncertainty is the reported uncertainty from NPL.

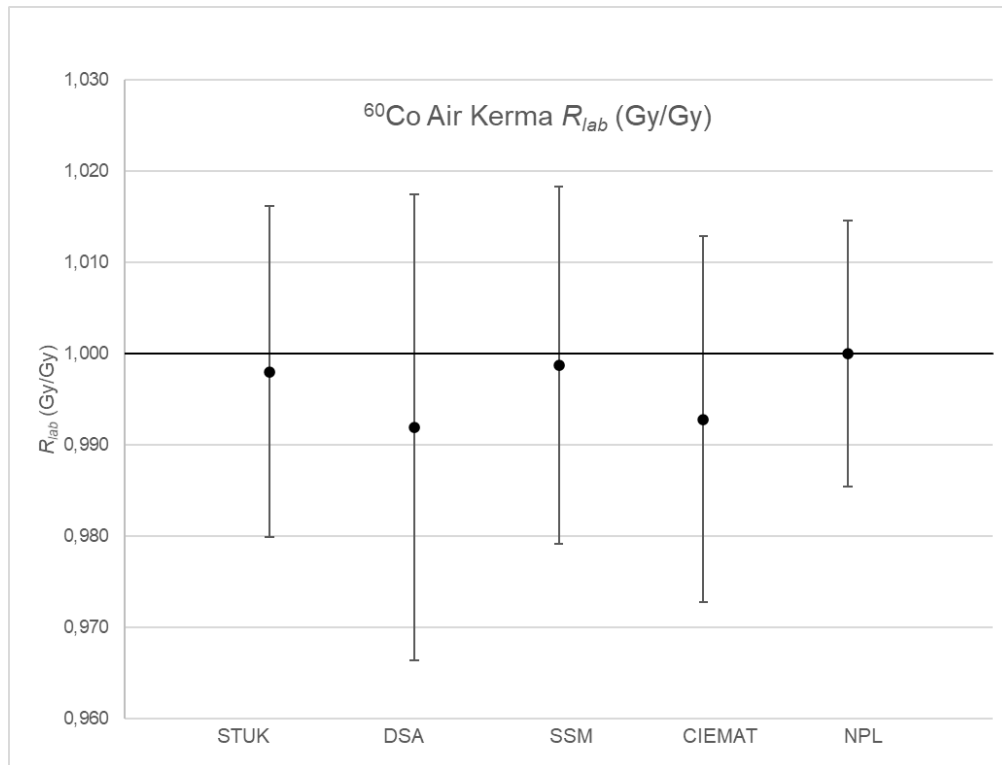

**Figure 2.** Graphical representation of the results in table 6: Ratios of calibration coefficients ( $R_{lab}$ ) and their expanded uncertainties ( $U_{lab}$ ,  $k = 2$ ) for participating laboratories in terms of air kerma for  $^{60}\text{Co}$  radiation quality.

#### 4. Discussion and conclusions

A supplementary comparison in terms of air kerma for  $^{241}\text{Am}$  and  $^{60}\text{Co}$  radiation has been carried out between five laboratories using two ionisation chambers as transfer standards. The comparison started with three transfer chambers, but one transfer chamber was excluded due to excessive and unpredictable leakage currents. The comparison results of all participating laboratories are in agreement within the expanded uncertainties and support the CMCs of the participating laboratories. The values presented here are in good agreement with earlier comparison results of the participating laboratories.

## 5. References

Bass, G A; Duane, S; Homer, M J; Kelly, M; Manning, J W; Maughan, D J; Nutbrown, R F; Sander, T; Shipley, D R; Snaith, J A D (2019a): *The NPL Air Kerma Primary Standard PS5-1/PS5-2 for  $^{137}\text{Cs}$  and  $^{60}\text{Co}$ : Summary of Factors Including ICRU 90 Recommendations*. NPL Report. IR 53

Bass, G A; Duane, S; Kelly, M; Manning, J W; Maughan, D J; Nutbrown, R F; Sander, T; Shipley, D R: *The NPL Air Kerma Primary Standard Free-Air Chamber for Medium Energy X-rays: Summary of Factors Incorporating ICRU Report 90 Recommendations*. NPL Report. IR 54, 2019b

Cornejo Díaz N. A., New LMRI-CIEMAT primary standard for  $^{137}\text{Cs}$  air-kerma. Measurement 188 (110374) 2022.

Cornejo Díaz N, García Mulas C, Avilés Lucas P, Embid Segura M, Respuesta relativa de la cámara de ionización PTW 32002 (00345) a la calidad del  $^{60}\text{Co}$  respecto a la calidad del  $^{137}\text{Cs}$  para la magnitud kerma en aire. DT-LMRI-2402. CIEMAT, 2024.

ICRU85a, ICRU report 85a (revised), Fundamental Quantities and Units for Ionizing Radiation, <https://www.icru.org/report/fundamental-quantities-and-units-for-ionizing-radiation-icru-report-85a-revised/>

ICRU90, ICRU Report 90, Key Data For Ionizing-Radiation Dosimetry: Measurement Standards And Applications, <https://www.icru.org/report/icru-report-90-key-data-for-ionizing-radiation-dosimetry-measurement-standards-and-applications/>

ISO 4037-1:2019 Radiological protection X and gamma reference radiation for calibrating dosimeters and doserate meters and for determining their response as a function of photon energy. Part 1: Radiation characteristics and production methods

ISO 4037-2:2019 X and gamma reference radiation for calibrating dosimeters and doserate meters and for determining their response as a function of photon energy  
Part 2: Dosimetry for radiation protection over the energy ranges from 8 keV to 1,3 MeV and 4 MeV to 9 MeV

JCGM (Joint Committee for Guides in Metrology). Evaluation of measurement data – Guide to the expression of uncertainty in measurement. JCGM 100:2008, GUM 1995 with minor corrections. First edition, September 2008.

KCDB, technical protocol <https://www.bipm.org/kcdb/comparison>

Kessler C., Roger P. and Cornejo Díaz N., Key comparison BIPM.RI(I)-K5 of the air-kerma standards of the CIEMAT, Spain and the BIPM in  $^{137}\text{Cs}$  gamma radiation. Metrologia 61 2024.

## 6. Appendix 1

Measurement results, uncertainty budgets and additional information for participating laboratories in the same order as the comparison measurements were performed:

STUK  $^{241}\text{Am}$ , STUK  $^{60}\text{Co}$ ; page 12-14

DSA  $^{241}\text{Am}$ , DSA  $^{60}\text{Co}$ ; page 15-19

NPL  $^{241}\text{Am}$ , NPL  $^{60}\text{Co}$ ; page 20-223

SSM  $^{241}\text{Am}$ , SSM  $^{60}\text{Co}$ ; page 24-28

CIEMAT  $^{60}\text{Co}$ ; page 29-36

STUK <sup>241</sup>Am

| Chamber   | EXRADIN A6 (XQ200282)                                | PTW 32003 (000296)                                   |
|---|--|--|
|   | <i>N<sub>Kair</sub></i>                              | <i>N<sub>Kair</sub></i>                              |
| Date of measurement   | Aug 2024   | Aug 2024   |
| Calibration coefficient [Gy/C]  | 36820  | 3020   |
| <i>U</i> ( <i>k</i> = 2) [%]  | 4,33   | 4,33   |
| mean ionization current [pA]  | -0,032   | -0,385   |
| measured leakage current [fA]   | -2,0   | -12  |
| Environmental conditions (T, p, h), is there correction for humidity? | 20 °C, 100.8 kPa, 50% rh, no correction for humidity | 20 °C, 100.8 kPa, 50% rh, no correction for humidity |
| Correction factors: <i>k<sub>elec</sub></i>                           | 1,0041   | 1,0041   |

| Background information                                 | <i>K<sub>air</sub></i>   |
|--|--|
| Radiation source                                       | <b>Am-241</b>  |
| Irradiator   | Custom made  |
| Field size   | 67 cm (95%)  |
| Dose rate [mGy/s]                                      | 1,16E-09   |
| SDD [cm]   | 200 cm   |
| Reference standard (chamber + traceability)            | PTW TM32002-0260, NPL  |
| Electrometer (charge vs current, range + traceability) | Keithley 6517B 4132822, measuring charge, 20 nC, VTT MIKES (Finland 11/21) |

Equation/model

$$NK = K(\text{air}) / ((I_{\text{tot}} - I_{\text{leak}}) * k(Tp) * k(\text{elec}))$$

Computation method (analytic or MC) and program model

Analytic

Quantity

K<sub>air</sub>

| Air kerma  | Type A                 | Type B       |
|--|------------------------|--------------|
|  | <i>Uncertainty (%)</i> |              |
| <b>1 Reference standard, set-up and radiation field</b>                              |                        |              |
| Calibration coefficient by PSDL  |                        | 0,85         |
| Long term stability of reference standard  |                        | 0,29         |
| Spectral difference of SSDL and PSDL   |                        | 0,29         |
| Difference in radial non-uniformity of the beam and field size                       |                        | 0,29         |
| <b>Combined uncertainty of reference standard and setup</b>                          | <b>0,00</b>            | <b>0,99</b>  |
| <b>2 Use of reference standard</b>   |                        |              |
| Chamber positioning (distance, orientation)  |                        |              |
| Current/charge measurement including leakage   | 0,05                   | 1,340        |
| Air temperature correction   |                        | 0,057        |
| Air pressure correction  |                        | 0,007        |
| Others (e.g. humidity of the measurement environment))                               |                        | 0,06         |
| <b>Combined uncertainty in measuring with reference standard</b>                     | <b>0,05</b>            | <b>1,34</b>  |
| <b>Combined uncertainty in air kerma determination, <i>K<sub>std</sub></i> (1+2)</b> | <b>0,05</b>            | <b>1,666</b> |
| <b>3 Use of transfer chamber</b>   |                        |              |
| Chamber positioning (distance, orientation)  |                        | 0,12         |
| Current/charge measurement including leakage   | 0,05                   | 1,340        |
| Air temperature correction   |                        | 0,057        |

|   |              |             |
|---|--------------|-------------|
| Air pressure correction   |              | 0,007       |
| Difference in radial non-uniformity of the beam and field size  |              | 0,29        |
| Decay of Am-241   |              |             |
| Others (e.g. humidity in measurement environment)   |              | 0,06        |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,05</b>  | <b>1,38</b> |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,07</b>  | <b>2,16</b> |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>2,164</b> |             |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>4,33</b>  |             |
| <b>Confidence level (%)</b>   | <b>95,3</b>  |             |

STUK  $^{60}\text{Co}$ 

| Chamber   | EXRADIN A6 (XQ200282)   | PTW 32003 (000296)                                   |
|---|---|--|
|   | $N_{kair}$  | $N_{kair}$   |
| Date of measurement   | Aug 2024  | Aug 2024   |
| Calibration coefficient [Gy/C]  | 3,692E+04   | 3,025E+03  |
| $U(k = 2)$ [%]  | <b>1,09</b>   | <b>1,09</b>  |
| mean ionization current [pA]  | -100,30   | -302,48  |
| measured leakage current [fA]   | -2,0  | -12  |
| Environmental conditions (T, p, h), is there correction for humidity? | 20 °C, 100.8 kPa, 50% rh, no correction for humidity                        | 20 °C, 100.8 kPa, 50% rh, no correction for humidity |
| Correction factors: $k_{elec}$  | 1,0041  | 1,0041   |
| <b>Background information</b>   |   |  |
|   | $K_{air}$   |  |
| Radiation source  | Co-60   |  |
| Irradiator  | Gemini  |  |
| Field size  | A6: 30 cm (98%) PTW: 60 cm (98%)  |  |
| A6 Dose rate [mGy/s]  | 3,70E-06  |  |
| A6 SDD [cm]   | 200 cm  |  |
| PTW Dose rate [Gy/s]  | 9,15E-07  |  |
| PTW SDD [cm]  | 400 cm  |  |
| Reference standard (chamber + traceability)                           | PTW TM32002-0260, PTB   |  |
| Electrometer (charge vs current, range + traceability)                | Keithley 6517B 4132822, measuring charge, 20 nC, VTT MIKES (Finland, 11/21) |  |

Equation/model

 $NK=K(\text{air})/((I_{\text{tot}}-I_{\text{leak}})*k(kTp)*k(\text{elec}))$ 

Computation method (analytic or MC) and program model

Analytic

Quantity

 $K_{\text{air}}$ 

| Air kerma   | Type A                 | Type B       |
|---|------------------------|--------------|
|   | <i>Uncertainty (%)</i> |              |
| <b>1 Reference standard, set-up and radiation field</b>   |                        |              |
| Calibration coefficient by PSDL   |                        | 0,375        |
| Long term stability of reference standard   |                        | 0,29         |
| Spectral difference of SSDL and PSDL  |                        | 0,03         |
| Difference in radial non-uniformity of the beam and field size  |                        | 0,06         |
| <b>Combined uncertainty of reference standard and setup</b>   | <b>0,00</b>            | <b>0,478</b> |
| <b>2 Use of reference standard</b>  |                        |              |
| Chamber positioning (distance, orientation)   |                        |              |
| Current/charge measurement including leakage  | 0,05                   | 0,124        |
| Air temperature correction  |                        | 0,06         |
| Air pressure correction   |                        | 0,01         |
| Others (e.g. humidity of the measurement environment))  |                        | 0,06         |
| <b>Combined uncertainty in measuring with reference standard</b>  | <b>0,05</b>            | <b>0,15</b>  |
| <b>Combined uncertainty in air kerma determination, <math>K_{\text{std}}</math> (1+2)</b>                                     | <b>0,05</b>            | <b>0,501</b> |
| <b>3 Use of transfer chamber</b>  |                        |              |
| Chamber positioning (distance, orientation)   |                        | 0,12         |
| Current/charge measurement including leakage  | 0,05                   | 0,124        |
| Air temperature correction  |                        | 0,057        |
| Air pressure correction   |                        | 0,007        |
| Difference in radial non-uniformity of the beam and field size  |                        | 0,06         |
| Decay of Co-60  |                        |              |
| Others (e.g. humidity in measurement environment)   |                        | 0,06         |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,05</b>            | <b>0,20</b>  |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,07</b>            | <b>0,539</b> |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>0,544</b>           |              |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>1,09</b>            |              |
| <b>Confidence level (%)</b>   | <b>95,3</b>            |              |

DSA <sup>241</sup>Am

| Chamber   | EXRADIN A6 (XQ200282)  | PTW 32003 (000296)  |
|---|--|---|
|   | <i>N<sub>Kair</sub></i>  | <i>N<sub>Kair</sub></i>   |
| Date of measurement   | 04.09.2024 to 05.09.2024   | 2024-09-09  |
| Calibration coefficient [ $\mu\text{Gy/nC}$ ]                         | 36,53  | 3,008   |
| <i>U</i> ( <i>k</i> = 2) [%]  | 1,74   | 1,89  |
| mean ionization current [A]   | -1,112E-12   | -2,107E-12  |
| measured leakage current [A]  | -1,3E-14   | -3,3E-14  |
| Environmental conditions (T, p, h), is there correction for humidity? | 04.09: T=294.60 K, P=100.83 kPa, h=65%, no correction for humidity | 09.09: T=294.15 K, P=98.38 kPa, h=68%, no correction for humidity |
| Environmental conditions (T, p, h), is there correction for humidity? | 05.09: T=294.25 K, P=101.39 kPa, h=63%, no correction for humidity | 09.09: T=294.17 K, P=98.28 kPa, h=70%, no correction for humidity |
| Correction factors: <i>k<sub>elec</sub></i>                           | Ref: 1.0009, UUT: 1.001  | Ref: 1.0009, UUT: 1.001   |
| Correction factors: <i>k<sub>TP</sub></i>                             | 04.09: Mean 1.010  | 09.09: Mean 1.033   |
| Correction factors: <i>k<sub>TP</sub></i>                             | 05.09: Mean 1.003  | 09.09: Mean 1.035   |

| Background information                                 | <i>K<sub>air</sub></i>   |
|--|--|
| Radiation source                                       | Am-241   |
| Irradiator   | DIR101, Veenstra   |
| Field size   | 24 cm for Exradin A6 chambers, 60 cm for the PTW chamber   |
| Dose rate [ $\mu\text{Gy/h}$ ] 100.0 cm                | 145  |
| Dose rate [ $\mu\text{Gy/h}$ ] 250.0 cm                | 22,4   |
| SDD [cm]   | 100.0 for Exradin A6 chambers, 250.0 for the PTW chamber   |
| Reference standard (chamber + traceability)            | Exradin A6 XQ102232, VSL 2016, for N-80  |
| Electrometer (charge vs current, range + traceability) | Keithley 6517A 0863876 and Keithley 6517A 0925329, measuring current, calibrated in-house and traceable to Justervesenet |
| other remarks  | All currents and dose rates are referenced to 01.09.2024   |

Exradin A6 XQ200282

## Quantity

K<sub>air</sub>

| Air kerma  | Type A                 | Type B      |
|--|------------------------|-------------|
|  | <i>Uncertainty (%)</i> |             |
| <b>1 Reference standard, set-up and radiation field</b>        |                        |             |
| Calibration coefficient by PSDL                                |                        | 0,80        |
| Long term stability of reference standard                      |                        | 0,10        |
| Spectral difference of SSDL and PSDL                           |                        | 0,20        |
| Difference in radial non-uniformity of the beam and field size |                        | 0,10        |
| <b>Combined uncertainty of reference standard and setup</b>    | <b>0,00</b>            | <b>0,84</b> |
| <b>2 Use of reference standard</b>                             |                        |             |
| Chamber positioning (distance, orientation)                    | 0,10                   |             |
| Current/charge measurement including leakage                   | 0,10                   |             |
| Air temperature correction                                     |                        | 0,06        |
| Air pressure correction  |                        | 0,02        |

|   |              |             |
|---|--------------|-------------|
| Others (e.g. humidity of the measurement environment))  |              | 0,02        |
| <b>Combined uncertainty in measuring with reference standard</b>  | <b>0,14</b>  | <b>0,07</b> |
| <b>Combined uncertainty in air kerma determination, <math>K_{std}</math> (1+2)</b>  | <b>0,14</b>  | <b>0,84</b> |
| <b>3 Use of transfer chamber</b>  |              |             |
| Chamber positioning (distance, orientation)   | 0,10         |             |
| Current/charge measurement including leakage  | 0,10         |             |
| Air temperature correction  |              | 0,06        |
| Air pressure correction   |              | 0,02        |
| Difference in radial non-uniformity of the beam and field size  |              |             |
| Decay of Am-241   |              | 0,00        |
| Others (e.g. humidity in measurement environment)   |              | 0,02        |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,14</b>  | <b>0,07</b> |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,20</b>  | <b>0,84</b> |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>0,865</b> |             |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>1,74</b>  |             |
| <b>Confidence level (%)</b>   | <b>95,3</b>  |             |

PTW TN32003, 000296

| Quantity   | Kair                   |             |
|--|------------------------|-------------|
|  | Type A                 | Type B      |
| <b>Air kerma</b>   |                        |             |
|  | <i>Uncertainty (%)</i> |             |
| <b>1 Reference standard, set-up and radiation field</b>                            |                        |             |
| Calibration coefficient by PSDL  |                        | 0,80        |
| Long term stability of reference standard  |                        | 0,10        |
| Spectral difference of SSDL and PSDL   |                        | 0,20        |
| Difference in radial non-uniformity of the beam and field size                     |                        | 0,10        |
| <b>Combined uncertainty of reference standard and setup</b>                        | <b>0,00</b>            | <b>0,84</b> |
| <b>2 Use of reference standard</b>   |                        |             |
| Chamber positioning (distance, orientation)  | 0,10                   |             |
| Current/charge measurement including leakage                                       | 0,40                   |             |
| Air temperature correction   |                        | 0,06        |
| Air pressure correction  |                        | 0,02        |
| Others (e.g. humidity of the measurement environment))                             |                        | 0,02        |
| <b>Combined uncertainty in measuring with reference standard</b>                   | <b>0,41</b>            | <b>0,07</b> |
| <b>Combined uncertainty in air kerma determination, <math>K_{std}</math> (1+2)</b> | <b>0,41</b>            | <b>0,84</b> |
| <b>3 Use of transfer chamber</b>   |                        |             |
| Chamber positioning (distance, orientation)  | 0,10                   |             |
| Current/charge measurement including leakage                                       | 0,06                   |             |
| Air temperature correction   |                        | 0,06        |
| Air pressure correction  |                        | 0,02        |
| Difference in radial non-uniformity of the beam and field size                     |                        |             |
| Decay of Am-241  |                        | 0,00        |
| Others (e.g. humidity in measurement environment)                                  |                        | 0,02        |
| <b>Combined uncertainty in measuring with transfer chamber</b>                     | <b>0,12</b>            | <b>0,07</b> |

|   |       |      |
|---|-------|------|
| Relative combined standard uncertainty (1+2+3)  | 0,43  | 0,84 |
| $U$ , Total relative measurement uncertainty for the air kerma calibration coefficient, $1\sigma$ | 0,945 |      |
| $U$ , Relative expanded measurement uncertainty, $k = 2$  | 1,89  |      |
| Confidence level (%)  | 95,3  |      |

## DSA $^{60}\text{Co}$

| Chamber   | EXRADIN A6 (XQ200282)  | PTW 32003 (000296)  |
|---|--|---|
|   | $N_{Kair}$   | $N_{Kair}$  |
| Date of measurement   | 04.09.2024 to 05.09.2024   | 09.09.2024 to 10.09.2024  |
| Calibration coefficient [ $\mu\text{Gy/nC}$ ]                         | 36,63  | 3,012   |
| $U(k = 2)$ [%]  | 1,94   | 2,33  |
| mean ionization current [ $\text{pA}$ ]                               | -1,267E-13   | -2,509E-13  |
| measured leakage current [ $\text{fA}$ ]                              | -1,1E-14   | -3,1E-14  |
| Environmental conditions (T, p, h), is there correction for humidity? | 04.09: T=294.59 K, P=100.85 kPa, h=65%, no correction for humidity | 09.09: T=294.17 K, P=98.34 kPa, h=69%, no correction for humidity |
| Environmental conditions (T, p, h), is there correction for humidity? | 05.09: T=294.34 K, P=101.36 kPa, h=64%, no correction for humidity | 10.09: T=294.64 K, P=97.66 kPa, h=47%, no correction for humidity |
| Correction factors: $k_{elec}$  | Ref: 1.0009, UUT: 1.001  | Ref: 1.0009, UUT: 1.001   |
| Correction factors: $k_{TP}$  | 04.09: Mean 1.010  | 09.09: Mean 1.034   |
| Correction factors: $k_{TP}$  | 05.09: Mean 1.004  | 10.09: Mean 1.043   |

| Background information                                 | $K_{air}$  |
|--|--|
| Radiation source                                       | <b>Co-60</b>   |
| Irradiator   | DIR101, Veenstra   |
| Field size   | 24 cm for Exradin A6 chambers, 60 cm for the PTW chamber   |
| Dose rate [ $\mu\text{Gy/h}$ ] 100.0 cm                | 15,3   |
| Dose rate [ $\mu\text{Gy/h}$ ] 250.0 cm                | 2,4  |
| SDD [cm]   | 100.0 for Exradin A6 chambers, 250.0 for the PTW chamber   |
| Reference standard (chamber + traceability)            | Exradin A6 XQ102232, IAEA 2023, for S-Cs and S-Co  |
| Electrometer (charge vs current, range + traceability) | Keithley 6517A 0863876 and Keithley 6517A 0925329, measuring current, calibrated in-house and traceable to Justervesenet |
| other remarks  | All currents and dose rates are referenced to 01.09.2024   |

Exradin A6 XQ200282

### Quantity

K<sub>air</sub>

| Air kerma  | Type A          | Type B |
|--|-----------------|--------|
|  | Uncertainty (%) |        |
| 1 Reference standard, set-up and radiation field |                 |        |

|   |              |              |
|---|--------------|--------------|
| Calibration coefficient by PSDL   |              | 0,40         |
| Long term stability of reference standard   |              | 0,10         |
| Spectral difference of SSDL and PSDL  |              | 0,05         |
| Difference in radial non-uniformity of the beam and field size  |              | 0,10         |
| <b>Combined uncertainty of reference standard and setup</b>   | <b>0,00</b>  | <b>0,43</b>  |
| <b>2 Use of reference standard</b>  |              |              |
| Chamber positioning (distance, orientation)   | 0,10         |              |
| Current/charge measurement including leakage  | 0,60         |              |
| Air temperature correction  |              | 0,06         |
| Air pressure correction   |              | 0,02         |
| Others (e.g. humidity of the measurement environment))  |              | 0,02         |
| <b>Combined uncertainty in measuring with reference standard</b>  | <b>0,61</b>  | <b>0,07</b>  |
| <b>Combined uncertainty in air kerma determination, <math>K_{std}</math> (1+2)</b>  | <b>0,61</b>  | <b>0,432</b> |
| <b>3 Use of transfer chamber</b>  |              |              |
| Chamber positioning (distance, orientation)   | 0,10         |              |
| Current/charge measurement including leakage  | 0,60         |              |
| Air temperature correction  |              | 0,06         |
| Air pressure correction   |              | 0,02         |
| Difference in radial non-uniformity of the beam and field size  |              |              |
| Decay of Co-60  |              | 0,00         |
| Others (e.g. humidity in measurement environment)   |              | 0,02         |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,61</b>  | <b>0,07</b>  |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,86</b>  | <b>0,44</b>  |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>0,965</b> |              |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>1,94</b>  |              |
| <b>Confidence level (%)</b>   | <b>95,3</b>  |              |

PTW TN32003, 000296

**Quantity**K<sub>air</sub>

| Air kerma  | K <sub>air</sub>       |             |
|--|------------------------|-------------|
|  | Type A                 | Type B      |
|  | <i>Uncertainty (%)</i> |             |
| <b>1 Reference standard, set-up and radiation field</b>  |                        |             |
| Calibration coefficient by PSDL  |                        | 0,40        |
| Long term stability of reference standard  |                        | 0,10        |
| Spectral difference of SSDL and PSDL   |                        | 0,05        |
| Difference in radial non-uniformity of the beam and field size   |                        | 0,10        |
| <b>Combined uncertainty of reference standard and setup</b>  | <b>0,00</b>            | <b>0,43</b> |
| <b>2 Uncertainty in the determination of kerma at 2.5 m based on historical data and measurements at other distances and interpolation</b> |                        |             |
|  |                        | 1,00        |
|  |                        |             |
|  |                        |             |
|  |                        |             |

|   |              |              |
|---|--------------|--------------|
| <b>Combined uncertainty in measuring with reference standard</b>  | <b>0,00</b>  | <b>1,00</b>  |
| <b>Combined uncertainty in air kerma determination, <math>K_{std}</math> (1+2)</b>  | <b>0,00</b>  | <b>1,087</b> |
| <b>3 Use of transfer chamber</b>  |              |              |
| Chamber positioning (distance, orientation)   | 0,10         |              |
| Current/charge measurement including leakage  | 0,40         |              |
| Air temperature correction  |              | 0,06         |
| Air pressure correction   |              | 0,02         |
| Difference in radial non-uniformity of the beam and field size  |              |              |
| Decay of Co-60  |              | 0,00         |
| Others (e.g. humidity in measurement environment)   |              | 0,02         |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,41</b>  | <b>0,07</b>  |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,41</b>  | <b>1,09</b>  |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>1,165</b> |              |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>2,33</b>  |              |
| <b>Confidence level (%)</b>   | <b>95,3</b>  |              |

NPL  $^{241}\text{Am}$ 

| Chamber   | EXRADIN A6 (XQ200282)   | PTW 32003 (000296)  |
|---|---|---|
|   | $N_{\text{Kair}}$   | $N_{\text{Kair}}$   |
| Date of measurement   | 04-Oct-24   | 04-Oct-24   |
| Calibration coefficient [Gy/C]  | 3,688E+04   | 3,035E+03   |
| $U(k=2)$ [%]  | 2,04  | 2,04  |
| mean ionization current [pA]  | -1,845  | -5,743  |
| measured leakage current [fA]   | -9  | 36  |
| Environmental conditions (T, p, h), is there correction for humidity? | T= 293.22 K (20.07C), p= 101.94 kPa, rh=50.2%, no correction for humidity | T= 293.22 K (20.07C), p= 101.94 kPa, rh=50.2%, no correction for humidity |
| Correction factors: $k_{\text{elec}}$                                 | 1,00  | 1,00  |

| Background information                                 | $K_{\text{air}}$   | $K_{\text{air}}$   |
|--|--|--|
| Radiation source                                       | Am-241   | Am-241   |
| Irradiator   | Mainance   | Mainance   |
| Field size (cm)  | 38,0   | 76,0   |
| Dose rate [uGy/h]                                      | 242,9  | 62,56  |
| SDD [cm]   | 100  | 200  |
| Reference standard (chamber + traceability)            | 2551/053 via specially constructed graphite walled ionization chamber to NPL 300 kV PS FAC | 2551/053 via specially constructed graphite walled ionization chamber to NPL 300 kV PS FAC |
| Electrometer (charge vs current, range + traceability) | Keithley 6517B measuring current, 20pA range, internal UKAS calibration                    | Keithley 6517B measuring current, 20pA range, internal UKAS calibration                    |
| other remarks- SNR                                     | 0,47%  | -0,63%   |

Table 1 Uncertainties in the primary standard factor

| Symbol                | Quantity, source of uncertainty  | Type A | Type B |
|-----------------------|--|--------|--------|
| $U_{\text{FAC-METS}}$ | Uncertainties in the 300 kV primary standard FAC correction factors, measurement, and calibration of a medium energy transfer standard | -      | 0,66   |
| $u_c(K_a)$            | Combined standard uncertainty  | 0,66   |        |

Uncertainties in the calibration of the low energy transfer standard

Table 2

| Symbol                 | Quantity, source of uncertainty           | Type A | Type B |
|------------------------|---|--------|--------|
| $U_{\text{METS-LETS}}$ | ME TS standard measurement uncertainty    | -      | 0,66   |
| $k_{\text{elec}}$      | Electrometer current calibration (pA/pA') | -      | 0,30   |
| $k_{\text{res}}$       | Electrometer resolution (nA)              | -      | 0,03   |
| $k_{\text{ion}}$       | Ion recombination correction              | 0,05   | -      |
| $I_{\text{leakage}}$   | Leakage current (A)                       | 0,10   | -      |
| $p$                    | Pressure (kPa)                            | 0,02   | -      |
| $T$                    | Temperature (K)                           | 0,04   | -      |
| $R_{\text{angular}}$   | Angular response change                   | 0,03   | -      |
| $R$                    | Repeatability                             | 0,30   | -      |



| <b>Table 1</b>                          |  | <b>Uncertainties in the primary standard factor</b> |        |
|---|--|---|--------|
| Symbol                                  | Quantity, source of uncertainty  | Type A  | Type B |
| $\bar{S}_{air}^{graphite} \cdot k_{fl}$ | Mass stopping power ratio (graphite to air)<br>x fluence perturbation correction | -   | 0,08   |
| $(\mu_{en}/\rho)_{graphite}^{air}$      | Mass energy absorption coefficient ratio (air<br>to graphite)                    | -   | 0,10   |
| $k_{wall}$                              | Wall correction  | -   | 0,10   |
| $u_c(\bar{F})$                          | Standard uncertainty   | 0,11  | 0,16   |
| $u_c(\bar{F})$                          | Combined standard uncertainty  | 0,20  |        |
| $k_{an} \times k_{rn}$                  | Product of axial uniformity and radial<br>uniformity correction factors          | 0,16  | 0,10   |
| $k_{stem}$                              | Stem scatter correction  | 0,01  | 0,05   |
| $k_{pol}$                               | Polarity correction  | 0,01  | -      |
| $u_c(F)$                                | Combined standard uncertainty  | 0,28  |        |
| $(W_{air}/e)^*$                         | Energy per ion pair (J/C)  | -   | 0,35   |
| $g$                                     | Fraction of energy lost by bremsstrahlung  | -   | 0,02   |
| $k_h$                                   | Humidity correction  | -   | 0,05   |
| $\rho_{air}$                            | Density of dry air (kg/m <sup>3</sup> )  | -   | 0,01   |
| $V$                                     | Volume of cavity (cm <sup>3</sup> )  | -   | 0,01   |
| $u_c(N_k)$                              | Combined standard uncertainty  | 0,28  |        |

\*Due to correlated uncertainties between the stopping power ratio and  $W_{air}/e$ , the uncertainty in  $W_{air}/e$  has been included in the combined uncertainty for the product  $\bar{S}_{air}^{graphite} \cdot k_{fl}$

| <b>Table 2</b> |   | <b>Uncertainties in the primary standard measurement</b> |        |
|----------------|---|--|--------|
| Symbol         | Quantity, source of uncertainty           | Type A   | Type B |
| $N_k$          | Total primary standard correction         | -  | 0,28   |
| $k_{elec}$     | Electrometer current calibration (pA/pA') | -  | 0,30   |
| $k_{res}$      | Electrometer resolution (nA)              | -  | 0,03   |
| $k_{ion}$      | Ion recombination correction              | 0,05   | -      |
| $I_{leakage}$  | Leakage current (A)                       | 0,10   | -      |
| $p$            | Pressure (kPa)                            | 0,02   | -      |
| $T$            | Temperature (K)                           | 0,04   | -      |
| $R_{angular}$  | Angular response change                   | 0,03   | -      |
| $R$            | Repeatability                             | 0,30   | -      |
| $u_c(K_a)$     | Combined standard uncertainty             | 0,53   |        |

| <b>Table 3</b> |   | <b>Uncertainties in the calibration of the NPL transfer standard</b> |        |
|----------------|---|--|--------|
| Symbol         | Quantity, source of uncertainty           | Type A   | Type B |
| $K_a$          | Air kerma rate                            | -  | 0,53   |
| $k_{elec}$     | Electrometer current calibration (nA/nA') | -  | 0,15   |
| $k_{res}$      | Electrometer resolution (nA)              | -  | 0,03   |
| $k_{ion}$      | Ion recombination correction              | 0,05   | -      |
| $I_{leakage}$  | Leakage current (A)                       | 0,10   | -      |
| $p$            | Pressure (kPa)                            | 0,02   | -      |
| $T$            | Temperature (K)                           | 0,04   | -      |
| $k_{dist}$     | Distance from source                      | -  | 0,05   |
| $k_{orient}$   | Orientation of chamber                    | -  | 0,01   |
| $R$            | Repeatability                             | 0,30   | -      |
| $u_c(N_k)$     | Combined standard uncertainty             | 0,64   |        |



# SSM <sup>241</sup>Am

| Chamber   | EXRADIN A6 (XQ200282)   | PTW 32003 (000296)   |
|---|---|--|
|   | <i>N<sub>kair</sub></i>   | <i>N<sub>kair</sub></i>                                    |
| Date of measurement   | 2024-11-15  | 2024-11-15   |
| Calibration coefficient [Gy/C]  | 36870   | 3042   |
| <i>U</i> ( <i>k</i> = 2) [%]  | 2,1   | 2,2  |
| mean ionization current [pA]  | -1,08   | -3,24  |
| measured leakage current [fA]   | 2,3   | -14,9  |
| Environmental conditions (T, p, h), is there correction for humidity? | T=21,45°C, p=101,62 kPa, rh=44% no correction for humidity                          | T=21,48°C, p=101,34 kPa, rh=44% no correction for humidity |
| Correction factors: <i>k<sub>elec</sub></i>                           | 1,00  | 1,00   |
| <b>Background information</b>   |   |  |
|   | <i>K<sub>air</sub></i>  |  |
| Radiation source  | <b>Am-241</b>   |  |
| Irradiator  | Veenstra DIR101   |  |
| Field size  | FWHM= 40 cm   | FWHM= 80 cm  |
| Dose rate [mGy/s]   | 3,987E-05   | 9,854E-06  |
| SDD [cm]  | 100   | 200  |
| Reference standard (chamber + traceability)                           | Exradin A6 XQ023361, NPL 2020100174   |  |
| Electrometer (charge vs current, range + traceability)                | Keysight B2987A-MY54321271, current measurements, 2E-12 och 2E-11 range, RISE 04/24 |  |
| other remarks   | radiation field: ISO 4037   |  |

### Equation/model

$$\Delta K_{1m} = \delta N_{k,PSDL} * \Delta I * \Delta k_{T,p} * \delta T * \delta k_{pos.jonk.1m,inmätning} * \delta k_{rek,1m} * \delta E_{PSDL} * \delta T^{1/2} * \delta k_{spridd} * \delta k_{fält} * \delta k_{stab} * \delta k_{spek}$$

$$\Delta K_{2m} = \delta N_{k,PSDL} * \Delta I * \Delta k_{T,p} * \delta T * \delta k_{pos.jonk.2m,inmätning} * \delta k_{rek,2m} * \delta E_{PSDL} * \delta T^{1/2} * \delta k_{spridd} * \delta k_{fält} * \delta k_{stab} * \delta k_{spek}$$

$$\Delta N_{k,1m} = \Delta K_{1m} * \delta k_{fält,instr,1m} * \delta k_{pos.instr,1m} * \Delta I_{Trans} * \Delta k_{T,p} * \delta T * \delta A * \delta RH * \delta k_{pos.källa} * \delta M_{1m} * \delta T^{1/2}$$

$$\Delta N_{k,2m} = \Delta K_{2m} * \delta k_{fält,instr,2m} * \delta k_{pos.instr,2m} * \Delta I_{Trans} * \Delta k_{T,p} * \delta T * \delta A * \delta RH * \delta k_{pos.källa} * \delta M_{Am,2m} * \delta T^{1/2}$$

Computation method (analytic or MC) and program model

analytic

### Chamber EXRADIN A6 (XQ200282)

#### Quantity

*K<sub>air</sub>*

| Air kerma  | Type A                 | Type B      |
|--|------------------------|-------------|
|  | <i>Uncertainty (%)</i> |             |
| <b>1 Reference standard, set-up and radiation field</b>        |                        |             |
| Calibration coefficient by PSDL                                |                        | 0,85        |
| Long term stability of reference standard                      |                        | 0,10        |
| Spectral difference of SSDL and PSDL                           |                        | 0,20        |
| Difference in radial non-uniformity of the beam and field size |                        | 0,01        |
| <b>Combined uncertainty of reference standard and setup</b>    | <b>0,00</b>            | <b>0,88</b> |
| <b>2 Use of reference standard</b>                             |                        |             |
| Chamber positioning (distance, orientation)                    |                        | 0,12        |
| Current/charge measurement including leakage                   | 0,340                  | 0,020       |
| Air temperature and pressure correction                        |                        | 0,04        |
| Scattering   |                        | 0,10        |

|   |              |              |
|---|--------------|--------------|
| Uncertainty in half-life  |              | 0,14         |
| Recombination   |              | 0,01         |
| Temperature gradients   |              | 0,06         |
| Others (e.g. humidity of the measurement environment))  |              | 0,02         |
| <b>Combined uncertainty in measuring with reference standard</b>  | <b>0,34</b>  | <b>0,22</b>  |
| <b>Combined uncertainty in air kerma determination, <math>K_{std}</math> (1+2)</b>  | <b>0,34</b>  | <b>0,907</b> |
| <b>3 Use of transfer chamber</b>  |              |              |
| Chamber positioning (distance, orientation)   |              | 0,12         |
| Current/charge measurement including leakage  | 0,03         | 0,020        |
| Air temperature and pressure correction   |              | 0,04         |
| Scattering  |              | 0,10         |
| Uncertainty in half-life  |              | 0,14         |
| Temperature gradients   |              | 0,06         |
| Difference in radial non-uniformity of the beam and field size  |              | 0,30         |
| Others (e.g. humidity in measurement environment)   |              | 0,02         |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,03</b>  | <b>0,37</b>  |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,34</b>  | <b>0,98</b>  |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>1,038</b> |              |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>2,08</b>  |              |
| <b>Confidence level (%)</b>   | <b>95,3</b>  |              |

## Camber PTW 32003 (000296)

## Quantity

Kair

| Air kerma  | Type A          | Type B       |
|--|-----------------|--------------|
|  | Uncertainty (%) |              |
| <b>1 Reference standard, set-up and radiation field</b>                            |                 |              |
| Calibration coefficient by PSDL  |                 | 0,85         |
| Long term stability of reference standard  |                 | 0,10         |
| Spectral difference of SSDL and PSDL   |                 | 0,20         |
| Difference in radial non-uniformity of the beam and field size                     |                 | 0,01         |
| <b>Combined uncertainty of reference standard and setup</b>                        | <b>0,00</b>     | <b>0,88</b>  |
| <b>2 Use of reference standard</b>   |                 |              |
| Chamber positioning (distance, orientation)  |                 | 0,06         |
| Current/charge measurement including leakage                                       | 0,500           | 0,020        |
| Air temperature and pressure correction  |                 | 0,04         |
| Scattering   |                 | 0,10         |
| Uncertainty in half-life   |                 | 0,14         |
| Recombination  |                 | 0,01         |
| Temperature gradients  |                 | 0,06         |
| Others (e.g. humidity of the measurement environment))                             |                 | 0,02         |
| <b>Combined uncertainty in measuring with reference standard</b>                   | <b>0,50</b>     | <b>0,20</b>  |
| <b>Combined uncertainty in air kerma determination, <math>K_{std}</math> (1+2)</b> | <b>0,50</b>     | <b>0,901</b> |
| <b>3 Use of transfer chamber</b>   |                 |              |
| Chamber positioning (distance, orientation)  |                 | 0,06         |

|  |              |             |
|--|--------------|-------------|
| Current/charge measurement including leakage   | 0,16         | 0,020       |
| Air temperature and pressure correction  |              | 0,04        |
| Scattering   |              | 0,10        |
| Uncertainty in half-life   |              | 0,14        |
| Temperature gradients  |              | 0,06        |
| Difference in radial non-uniformity of the beam and field size                                 |              | 0,20        |
| Others (e.g. humidity in measurement environment)  |              | 0,02        |
| <b>Combined uncertainty in measuring with transfer chamber</b>                                 | <b>0,16</b>  | <b>0,28</b> |
| <b>Relative combined standard uncertainty (1+2+3)</b>  | <b>0,53</b>  | <b>0,94</b> |
| <b>U, Total relative measurement uncertainty for the air kerma calibration coefficient, 1σ</b> | <b>1,081</b> |             |
| <b>U, Relative expanded measurement uncertainty, k = 2</b>                                     | <b>2,17</b>  |             |
| <b>Confidence level (%)</b>  | 95,3         |             |

### SSM <sup>60</sup>Co

| Chamber   | EXRADIN A6 (XQ200282)   | PTW 32003 (000296)   |
|---|---|--|
|   | <i>N<sub>Kair</sub></i>   | <i>N<sub>Kair</sub></i>                                    |
| Date of measurement   | 2024-11-15  | 2024-11-15   |
| Calibration coefficient [Gy/C]  | 36910   | 3030   |
| U (k = 2) [%]   | 1,3   | 1,4  |
| mean ionization current [pA]  | -0,063  | -0,192   |
| measured leakage current [fA]   | -2,0  | -15,8  |
| Environmental conditions (T, p, h), is there correction for humidity? | T=21,50°C, p=101,77 kPa, rh=44% no correction for humidity                | T=21,41°C, p=100,37 kPa, rh=43% no correction for humidity |
| Correction factors: k <sub>elec</sub>                                 | 1,00  | 1,00   |
| <b>Background information</b>   | <b>K<sub>air</sub></b>  |  |
| Radiation source  | Co-60   |  |
| Irradiator  | Veenstra DIR101   |  |
| Field size  | FWHM= 40 cm   | FWHM= 80 cm  |
| Dose rate [mGy/s]   | 2,346E-06   | 5,832E-07  |
| SDD [cm]  | 100   | 200  |
| Reference standard (chamber + traceability)                           | Exradin A6 XQ040063, BIPM 2016  |  |
| Electrometer (charge vs current, range + traceability)                | Keysight B2987A-MY54321271, current measurements, 2E-12 range, RISE 04/24 |  |
| other remarks   | radiation field: ISO 4037   |  |

Equation/model

$$\Delta K_{1m} = \delta N_{k,PSDL} \cdot \Delta I \cdot \Delta k_{T,p} \cdot \delta T \cdot \delta k_{pos.jonk.1m,inmätning} \cdot \delta k_{rek,1m} \cdot \delta E_{PSDL} \cdot \delta T_{1/2} \cdot \delta k_{spridd} \cdot \delta k_{fält} \cdot \delta k_{stab} \cdot \delta k_{spek}$$

$$\Delta K_{2m} = \delta N_{k,PSDL} \cdot \Delta I \cdot \Delta k_{T,p} \cdot \delta T \cdot \delta k_{pos.jonk.2m,inmätning} \cdot \delta k_{rek,2m} \cdot \delta E_{PSDL} \cdot \delta T_{1/2} \cdot \delta k_{spridd} \cdot \delta k_{fält} \cdot \delta k_{stab} \cdot \delta k_{spek}$$

$$\Delta N_{k,1m} = \Delta K_{1m} \cdot \delta k_{fält,instr,1m} \cdot \delta k_{pos.instr,1m} \cdot \Delta I_{trans} \cdot \Delta k_{T,p} \cdot \delta T \cdot \delta A \cdot \delta RH \cdot \delta k_{pos.käll} \cdot \delta M_{1m} \cdot \delta T_{1/2}$$

$$\Delta N_{k,2m} = \Delta K_{2m} * \delta k_{\text{fält, instr, 2m}} * \delta k_{\text{pos, instr, 2m}} * \Delta I_{\text{trans}} * \Delta k_{T,p} * \delta T * \delta A * \delta RH * \delta k_{\text{pos, källa}} * \delta M_{Am, 2m} * \delta T_{1/2}$$

Computation method (analytic or MC) and program model

analytic

**Chamber EXRADIN A6 (XQ200282)****Quantity**

Kair

| <b>Air kerma</b>  | <b>Type A</b>          | <b>Type B</b> |
|---|------------------------|---------------|
|   | <i>Uncertainty (%)</i> |               |
| <b>1 Reference standard, set-up and radiation field</b>   |                        |               |
| Calibration coefficient by PSDL   | 0,11                   | 0,13          |
| Long term stability of reference standard   |                        | 0,10          |
| Spectral difference of SSDL and PSDL  |                        | 0,20          |
| Difference in radial non-uniformity of the beam and field size  |                        | 0,01          |
| <b>Combined uncertainty of reference standard and setup</b>   | <b>0,11</b>            | <b>0,26</b>   |
| <b>2 Use of reference standard</b>  |                        |               |
| Chamber positioning (distance, orientation)   |                        | 0,12          |
| Current/charge measurement including leakage  | 0,40                   | 0,020         |
| Air temperature and pressure correction   |                        | 0,04          |
| Scattering  |                        | 0,10          |
| Uncertainty in half-life Co-60  |                        | 0,00          |
| Recombination   |                        | 0,01          |
| Temperature gradients   |                        | 0,06          |
| Others (e.g. humidity of the measurement environment))  |                        | 0,02          |
| <b>Combined uncertainty in measuring with reference standard</b>  | <b>0,40</b>            | <b>0,17</b>   |
| <b>Combined uncertainty in air kerma determination, <math>K_{\text{std}}</math> (1+2)</b>                                     | <b>0,41</b>            | <b>0,311</b>  |
| <b>3 Use of transfer chamber</b>  |                        |               |
| Chamber positioning (distance, orientation)   |                        | 0,12          |
| Current/charge measurement including leakage  | 0,02                   | 0,020         |
| Air temperature and pressure correction   |                        | 0,04          |
| Scattering  |                        | 0,10          |
| Uncertainty in half-life Co-60  |                        | 0,00          |
| Temperature gradients   |                        | 0,06          |
| Difference in radial non-uniformity of the beam and field size  |                        | 0,30          |
| Others (e.g. humidity in measurement environment)   |                        | 0,02          |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,02</b>            | <b>0,35</b>   |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,42</b>            | <b>0,47</b>   |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>0,624</b>           |               |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>1,25</b>            |               |
| <b>Confidence level (%)</b>   | <b>95,3</b>            |               |

**Chamber PTW 32003 (000296)****Quantity**

Kair

| <b>Air kerma</b>  | <b>Type A</b>          | <b>Type B</b> |
|---|------------------------|---------------|
|   | <i>Uncertainty (%)</i> |               |
| <b>1 Reference standard, set-up and radiation field</b> |                        |               |
| Calibration coefficient by PSDL                         | 0,11                   | 0,13          |
| Long term stability of reference standard               |                        | 0,10          |

|   |              |              |
|---|--------------|--------------|
| Spectral difference of SSDL and PSDL  |              | 0,20         |
| Difference in radial non-uniformity of the beam and field size  |              | 0,01         |
| <b>Combined uncertainty of reference standard and setup</b>   | <b>0,11</b>  | <b>0,26</b>  |
| <b>2 Use of reference standard</b>  |              |              |
| Chamber positioning (distance, orientation)   |              | 0,06         |
| Current/charge measurement including leakage  | 0,50         | 0,020        |
| Air temperature and pressure correction   |              | 0,04         |
| Scattering  |              | 0,10         |
| Uncertainty in half-life Co-60  |              | 0,00         |
| Recombination   |              | 0,01         |
| Temperature gradients   |              | 0,06         |
| Others (e.g. humidity of the measurement environment))  |              | 0,02         |
| <b>Combined uncertainty in measuring with reference standard</b>  | <b>0,50</b>  | <b>0,14</b>  |
| <b>Combined uncertainty in air kerma determination, <math>K_{std}</math> (1+2)</b>  | <b>0,51</b>  | <b>0,294</b> |
| <b>3 Use of transfer chamber</b>  |              |              |
| Chamber positioning (distance, orientation)   |              | 0,06         |
| Current/charge measurement including leakage  | 0,04         | 0,020        |
| Air temperature and pressure correction   |              | 0,04         |
| Scattering  |              | 0,30         |
| Uncertainty in half-life Co-60  |              | 0,02         |
| Temperature gradients   |              | 0,06         |
| Difference in radial non-uniformity of the beam and field size  |              | 0,20         |
| Others (e.g. humidity in measurement environment)   |              | 0,02         |
| <b>Combined uncertainty in measuring with transfer chamber</b>  | <b>0,04</b>  | <b>0,37</b>  |
| <b>Relative combined standard uncertainty (1+2+3)</b>   | <b>0,51</b>  | <b>0,48</b>  |
| <b><math>U</math>, Total relative measurement uncertainty for the air kerma calibration coefficient, <math>1\sigma</math></b> | <b>0,700</b> |              |
| <b><math>U</math>, Relative expanded measurement uncertainty, <math>k = 2</math></b>  | <b>1,40</b>  |              |
| <b>Confidence level (%)</b>   | <b>95,3</b>  |              |

CIEMAT  $^{60}\text{Co}$ 

| Chamber   | EXRADIN A6 (XQ200282)  | PTW 32003 (000296)  |
|---|--|---|
| Quantity  | $N_{Kair}$   | $N_{Kair}$  |
| Date of measurements  | 27/11/2024 - 19/12/2024  | 02/12/2024 - 18/12/2024   |
| Calibration coefficient [Gy/C]  | <b>3,6785E+04</b>  | <b>3,0042E+03</b>   |
| $U(k=2)$ [%]  | <b>1,40</b>  | <b>1,47</b>   |
| Mean ionization current [pA]  | -4,059   | -12,32  |
| measured leakage current [fA]   | 2,00   | 5,00  |
| Environmental conditions (T, p, h), is there correction for humidity? | $T = 292,22 \text{ K (19,07 } ^\circ\text{C)}$ , $P = 94,69 \text{ kPa}$ , $h = 41,2 \%$ . No correction applied for humidity. | $T = 291,69 \text{ K (18,54 } ^\circ\text{C)}$ , $P = 94,46 \text{ kPa}$ , $h = 38,5 \%$ . No correction applied for humidity.                      |
| Correction factors: $k_{elec}$  | 1,001 (HIGH, uncertainty included)   | 1,001 (HIGH, uncertainty included)  |
| Other remarks:  | -  | -   |
| <b>Background information</b>   |  |   |
|   | $K_{air}$  |   |
| Radiation source  | Co-60  |   |
| Irradiator  | NI-646 (Nuclear Ibérica)   |   |
| Field size  | Diameter: 36,8 cm  | Diameter: 73,7 cm   |
| Air Kerma rate [mGy/s]  | 1,4932E-04   | 3,6999E-05  |
| SDD [cm]  | 150  | 300   |
| Reference standard (chamber + traceability)                           | Graphite chambers CS-001 and SP-001 and secondary standards: 1-PTW 32005 (00047) and 2-PTW 32002 (00345). Traceability: CIEMAT | Graphite chambers CS-001 and SP-001 and secondary standards: 1-PTW 32005 (00047), 2-PTW 32002 (00345) and 3-PTW 32003 (00134). Traceability: CIEMAT |
| Electrometer (charge vs current, range + traceability)                | PTW UNIDOS - T10002-20641 (Charge mode, range HIGH (22 nC), VSL (Nederlands 05/2024))  | PTW UNIDOS - T10002-20641 (Charge mode, range HIGH (22 nC), VSL (Nederlands 05/2024))   |

Primary Reference (Measurement. Volume 188, 110374 (2022)) for  $^{137}\text{Cs}$  with a beam quality correction factor ( $k_{Co,Cs}$ ) applied to the calibration coefficient of the secondary standard PTW 32002 (CIEMAT Report: DT-LMRI-2402).

$$\dot{K}_{air} = \frac{I}{\rho_0 \cdot V_{col}} \cdot \left( \frac{\bar{W}}{e} \right)_{air} \cdot \left( \frac{\bar{S}_{el}}{\rho} \right)_{c,air} \cdot \left( \frac{\bar{\mu}_{en}}{\rho} \right)_{air,c} \cdot \frac{1}{(1 - \bar{g}_{air})} \cdot \prod_i k_i$$

$$\left\{ \prod_i k_i = k_{PT} \cdot k_h \cdot k_{dec} \cdot k_{att} \cdot k_{pos} \cdot k_{pol} \cdot k_s \cdot k_{st} \cdot k_{wall} \cdot k_{an} \cdot k_{rn} \cdot k_{SA} \right\}$$

$$N_{K,Co} = N_{K,Cs} \cdot k_{Co,Cs}$$

## EXRADIN A6 (XQ200282)

| <b>Table 1: Laboratory reference</b>                                       |                 |             |
|--|-----------------|-------------|
| Quantity: Air Kerma rate (137-Cs)  |                 |             |
| Uncertainty components   | Type A          | Type B      |
|  | Uncertainty (%) |             |
| Physical constants   |                 |             |
| $\rho_0$ (dry air density)   | -               | 0,01        |
| $(\bar{W}/e)_{\text{air}} \cdot (\bar{S}_{\text{el}}/\rho)_{\text{c,air}}$ | -               | 0,13        |
| $(\bar{\mu}_{\text{en}}/\rho)_{\text{air,c}} / (1 - \bar{g}_{\text{air}})$ | -               | 0,10        |
| Quadratic summation  | <b>0,00</b>     | <b>0,16</b> |
| Chamber volume and Correction factors                                      |                 |             |
| $V_{\text{col}}$ (Chamber collection volume)                               | -               | 0,10        |
| $k_{pT}$ (air pressure and temperature)                                    | -               | 0,07        |
| $k_h$ (humidity)   | -               | 0,03        |
| $k_{\text{dec}}$ (source decay)  | -               | 0,01        |
| $k_{\text{att}}$ (air attenuation)   | -               | 0,03        |
| $k_{\text{pos}}$ (chamber positioning)                                     | -               | 0,06        |
| $k_{\text{pol}}$ (effect of the polarizing voltage)                        | -               | 0,01        |
| $k_s$ (recombination losses)   | 0,01            | 0,02        |
| $k_{\text{st}}$ (stem scattering)  | 0,03            | -           |
| $k_{\text{wall}}$ (wall effect)  | 0,01            | 0,10        |
| $k_{\text{an}}$ (axial non-uniformity)                                     | 0,05            | 0,03        |
| $k_{\text{rn}}$ (radial non-uniformity)                                    | 0,06            | 0,08        |
| $k_{\text{SA}}$ (Spencer-Attix theory)                                     | -               | 0,10        |
| Quadratic summation  | <b>0,08</b>     | <b>0,22</b> |
| Ionization current measurements  |                 |             |
| Electrometer resolution  | -               | 0,01        |
| Leakage current  | -               | 0,03        |
| $N_{\text{el}}$ (Electrometer calibration factor)                          | -               | 0,10        |
| $f_{\text{non-lin}}$ (Linearity correction of the electrometer response)   | -               |             |
| $f_{\text{tem}}$ (rate of the electrometer timer)                          | -               | 0,10        |
| Repeatability  | 0,02            |             |
| Quadratic summation  | <b>0,02</b>     | <b>0,14</b> |
| Reference Air Kerma rate   |                 |             |
| Quadratic summation  | <b>0,09</b>     | <b>0,31</b> |
| Relative combined standard uncertainty, $u(\dot{K}_{\text{air}})$          | <b>0,32</b>     |             |

| <b>Table 2: Uncertainties in the calibration of the CIEMAT secondary standard 1 (30 cm<sup>3</sup>)</b> |                 |             |
|---|-----------------|-------------|
| Quantity: $N_{k,Cs}$ (Gy/C)   |                 |             |
| Uncertainty components  | Type A          | Type B      |
|   | Uncertainty (%) |             |
| Reference air kerma rate  | 0,09            | 0,31        |
| Measured current (including leakage)  | 0,01            | 0,12        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,06        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,03            | -           |
| Quadratic summation   | <b>0,09</b>     | <b>0,36</b> |
| Relative combined standard uncertainty, $u(N_{k,Cs})$   | <b>0,37</b>     |             |

| <b>Table 3: Uncertainties in the calibration of the CIEMAT secondary standard 2 (1000 cm<sup>3</sup>)</b> |                 |             |
|---|-----------------|-------------|
| Quantity: Air Kerma rate (Obtained with the secondary standard 1)   |                 |             |
| Uncertainty components  | Type A          | Type B      |
|   | Uncertainty (%) |             |
| Calibration coefficient of the secondary standard 1, $N_{k,Cs}$   | 0,09            | 0,36        |
| Measured current (including leakage correction)   | 0,02            | 0,11        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,06        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,02            | -           |
| Quadratic summation   | <b>0,10</b>     | <b>0,40</b> |
| Relative combined standard uncertainty, $u(\dot{K}_{air})$  | <b>0,41</b>     |             |
| Quantity: $N_{k,Co} = N_{k,Cs} \times k_{Co,Cs}$ (Gy/C)   |                 |             |
| Air kerma rate  | 0,10            | 0,40        |
| Beam Quality correction factor, $k_{Co,Cs}$   | -               | 0,40        |
| Measured current (including leakage correction)   | 0,01            | 0,12        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,06        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,09            | -           |
| Quadratic summation   | <b>0,13</b>     | <b>0,59</b> |
| Relative combined standard uncertainty, $u(N_{k,Co})$   | <b>0,61</b>     |             |

| Measurements in 60-Co beam  |                 |             |
|---|-----------------|-------------|
| Table 4: Uncertainties in the calibration of the transfer chamber (EXRADIN A6 (XQ200282)) |                 |             |
| Quantity: Air Kerma rate (Obtained with the secondary standard 2)                         |                 |             |
| Uncertainty components  | Type A          | Type B      |
|   | Uncertainty (%) |             |
| Calibration coefficient of the secondary standard 2, $N_{K,Co}$                           | 0,13            | 0,59        |
| Measured current (including leakage correction)   | 0,02            | 0,11        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,08        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,06            | -           |
| Quadratic summation   | <b>0,15</b>     | <b>0,62</b> |
| Relative combined standard uncertainty, $u(\dot{K}_{air})$                                | <b>0,64</b>     |             |
| Quantity: $N_{k,Co}$ (Gy/C)   |                 |             |
| Air kerma rate  | 0,15            | 0,62        |
| Measured current (including leakage correction)   | 0,02            | 0,12        |
| Ion recombination   | -               | 0,15        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,08        |
| Radial non-uniformity   | -               | 0,15        |
| Repeatability   | 0,11            | -           |
| Quadratic summation   | <b>0,18</b>     | <b>0,67</b> |
| Relative combined standard uncertainty ( $1\sigma$ ), $u(N_{k,Co})$                       | <b>0,70</b>     |             |
| <b>Relative expanded uncertainty (<math>k = 2</math>), <math>U(N_{k,Co})</math></b>       | <b>1,40</b>     |             |
| <b>Coverage probability (%)</b>   | <b>95</b>       |             |

## PTW 32003 (000296)

| <b>Table 1: Laboratory reference</b>                                       |                 |             |
|--|-----------------|-------------|
| Quantity: Air Kerma rate (137-Cs)  |                 |             |
| Uncertainty components   | Type A          | Type B      |
|  | Uncertainty (%) |             |
| Physical constants   |                 |             |
| $\rho_0$ (dry air density)   | -               | 0,01        |
| $(\bar{W}/e)_{\text{air}} \cdot (\bar{S}_{\text{el}}/\rho)_{\text{c,air}}$ | -               | 0,13        |
| $(\bar{\mu}_{\text{en}}/\rho)_{\text{air,c}} / (1 - \bar{g}_{\text{air}})$ | -               | 0,10        |
| Quadratic summation  | <b>0,00</b>     | <b>0,16</b> |
| Chamber volume and Correction factors                                      |                 |             |
| $V_{\text{col}}$ (Chamber collection volume)                               | -               | 0,10        |
| $k_{pT}$ (air pressure and temperature)                                    | -               | 0,07        |
| $k_h$ (humidity)   | -               | 0,03        |
| $k_{\text{dec}}$ (source decay)  | -               | 0,01        |
| $k_{\text{att}}$ (air attenuation)   | -               | 0,03        |
| $k_{\text{pos}}$ (chamber positioning)                                     | -               | 0,06        |
| $k_{\text{pol}}$ (effect of the polarizing voltage)                        | -               | 0,01        |
| $k_s$ (recombination losses)   | 0,01            | 0,02        |
| $k_{\text{st}}$ (stem scattering)  | 0,03            | -           |
| $k_{\text{wall}}$ (wall effect)  | 0,01            | 0,10        |
| $k_{\text{an}}$ (axial non-uniformity)                                     | 0,05            | 0,03        |
| $k_r$ (radial non-uniformity)  | 0,06            | 0,08        |
| $k_{\text{SA}}$ (Spencer-Attix theory)                                     | -               | 0,10        |
| Quadratic summation  | <b>0,08</b>     | <b>0,22</b> |
| Ionization current measurements  |                 |             |
| Electrometer resolution  | -               | 0,01        |
| Leakage current  | -               | 0,03        |
| $N_{\text{el}}$ (Electrometer calibration factor)                          | -               | 0,10        |
| $f_{\text{non-lin}}$ (Linearity correction of the electrometer response)   | -               |             |
| $f_{\text{tem}}$ (rate of the electrometer timer)                          | -               | 0,10        |
| Repeatability  | 0,02            |             |
| Quadratic summation  | <b>0,02</b>     | <b>0,14</b> |
| Reference Air Kerma rate   |                 |             |
| Quadratic summation  | <b>0,09</b>     | <b>0,31</b> |
| Relative combined standard uncertainty, $u(\dot{K}_{\text{air}})$          | <b>0,32</b>     |             |

| <b>Table 2: Uncertainties in the calibration of the CIEMAT secondary standard 1 (30 cm<sup>3</sup>)</b> |                 |             |
|---|-----------------|-------------|
| Quantity: $N_{k,Cs}$ (Gy/C)   |                 |             |
| Uncertainty components  | Type A          | Type B      |
|   | Uncertainty (%) |             |
| Reference air kerma rate  | 0,09            | 0,31        |
| Measured current (including leakage correction)   | 0,01            | 0,12        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,06        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,03            | -           |
| Quadratic summation   | <b>0,09</b>     | <b>0,36</b> |
| Relative combined standard uncertainty, $u(N_{k,Cs})$   | <b>0,37</b>     |             |

| <b>Table 3: Uncertainties in the calibration of the CIEMAT secondary standard 2 (1000 cm<sup>3</sup>)</b> |                 |             |
|---|-----------------|-------------|
| Quantity: Air Kerma rate (Obtained with the secondary standard 1)   |                 |             |
| Uncertainty components  | Type A          | Type B      |
|   | Uncertainty (%) |             |
| Calibration coefficient of the secondary standard 1, $N_{k,Cs}$   | 0,09            | 0,36        |
| Measured current (including leakage correction)   | 0,02            | 0,11        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,06        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,02            | -           |
| Quadratic summation   | <b>0,10</b>     | <b>0,40</b> |
| Relative combined standard uncertainty, $u(\dot{K}_{air})$  | <b>0,41</b>     |             |
| Quantity: $N_{k,Co} = N_{k,Cs} \times k_{Co,Cs}$ (Gy/C)   |                 |             |
| Air kerma rate  | 0,10            | 0,40        |
| Beam Quality correction factor, $k_{Co,Cs}$   | -               | 0,40        |
| Measured current (including leakage correction)   | 0,01            | 0,12        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,06        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,09            | -           |
| Quadratic summation   | <b>0,13</b>     | <b>0,59</b> |
| Relative combined standard uncertainty, $u(N_{k,Co})$   | <b>0,61</b>     |             |

| Measurements in 60-Co beam  |                 |             |
|---|-----------------|-------------|
| Table 4: Uncertainties in the calibration of the CIEMAT secondary standard 3 (10000 cm <sup>3</sup> ) |                 |             |
| Quantity: Air Kerma rate (Obtained with the secondary standard 2)                                     |                 |             |
| Uncertainty components  | Type A          | Type B      |
|   | Uncertainty (%) |             |
| Calibration coefficient of the transfer standard 2, $N_{K, Co}$                                       | 0,13            | 0,59        |
| Measured current (including leakage correction)   | 0,02            | 0,11        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,08        |
| Radial non-uniformity correction  | -               | 0,10        |
| Repeatability   | 0,06            | -           |
| Quadratic summation   | <b>0,15</b>     | <b>0,62</b> |
| Relative combined standard uncertainty, $u(\dot{K}_{air})$  | <b>0,64</b>     |             |
| Quantity: $N_{k, Co}$ (Gy/C)  |                 |             |
| Air kerma rate  | 0,15            | 0,62        |
| Measured current (including leakage correction)   | 0,01            | 0,12        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,08        |
| Radial non-uniformity   | -               | 0,10        |
| Repeatability   | 0,12            | -           |
| Quadratic summation   | <b>0,19</b>     | <b>0,65</b> |
| Relative combined standard uncertainty (1 $\sigma$ ), $u(N_{k, Co})$                                  | <b>0,67</b>     |             |

| <b>Table 5: Uncertainties in the calibration of the transfer chamber PTW 32003 (000296)</b> |                 |             |
|---|-----------------|-------------|
| Quantity: Air Kerma rate (Obtained with the secondary standard 3)                           |                 |             |
| Uncertainty components  | Type A          | Type B      |
|   | Uncertainty (%) |             |
| Calibration coefficient of the secondary standard 3, $N_{K, Co}$                            | 0,19            | 0,65        |
| Measured current (including leakage correction)   | 0,03            | 0,11        |
| Recombination correction  | -               | 0,05        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,04        |
| Radial non-uniformity correction  | -               | 0,05        |
| Repeatability   | 0,05            | -           |
| Quadratic summation   | <b>0,20</b>     | <b>0,66</b> |
| Relative combined standard uncertainty, $u(\dot{K}_{air})$                                  | <b>0,69</b>     |             |
| Quantity: $N_{K, Co}$ (Gy/C)  |                 |             |
| Air kerma rate  | 0,20            | 0,66        |
| Measured current (including leakage correction)   | 0,01            | 0,12        |
| Ion recombination   | -               | 0,15        |
| Atmospheric pressure correction   | -               | 0,03        |
| Air temperature correction  | -               | 0,02        |
| Humidity  | -               | 0,03        |
| Chamber positioning   | -               | 0,04        |
| Radial non-uniformity   | -               | 0,10        |
| Repeatability   | 0,08            | -           |
| Quadratic summation   | <b>0,21</b>     | <b>0,70</b> |
| Relative combined standard uncertainty (1 $\sigma$ ), $u(N_{K, Co})$                        | <b>0,73</b>     |             |
| Relative expanded uncertainty ( $k = 2$ ), $U(N_{K, Co})$                                   | <b>1,47</b>     |             |
| Coverage probability (%)  | <b>95</b>       |             |