

## CCQM-K115.2018

### Key Comparison Study on Peptide Purity - Hexapeptide of HbA0

#### Final Report

April 2022

#### Prepared by:

Ralf D. Josephs  
Bureau International des Poids et Mesures (BIPM)  
Sèvres, France

#### Coordinating laboratories:

Ralf D. Josephs\*, Qinde Liu<sup>+</sup>, Gustavo Martos\*, Magali Bedu\*, Adeline Daireaux\*, Tiphaine Choteau\*, Steven Westwood\*, Robert Wielgosz\*, Jintana Nammoonnoy\*<sup>‡</sup>, Wei Zhang\*<sup>#</sup>, Sharon Yong<sup>+</sup>, Hong Liu<sup>+</sup>, Yizhao Chen<sup>+</sup>, Cheng Yang Ng<sup>+</sup>, Ting Lu<sup>+</sup>, Juan Wang<sup>+</sup>, Ho Wah Leung<sup>+</sup>, Tang Lin Teo<sup>+</sup>, Xiaoyun Gong<sup>#</sup>, Xinhua Dai<sup>#</sup>, Wenqiang Xia<sup>#</sup>, Lulu Feng<sup>#</sup>, Jie Xie<sup>#</sup>, Tao Peng<sup>#</sup>, Xiang Fang<sup>#</sup>, Liqing Wu<sup>#</sup>, Chang Li<sup>#</sup>, Jiafeng Song<sup>#</sup>, Ming Li<sup>#</sup>, Hongmei Li<sup>#</sup>

\* Bureau International des Poids et Mesures (BIPM)  
Sèvres, France

<sup>+</sup> Health Sciences Authority (HSA)  
Singapore

<sup>#</sup> National Institute of Metrology (NIM)  
Beijing, China

<sup>‡</sup> Seconded to the BIPM by the National Institute of Metrology Thailand (NIM)  
Bangkok, Thailand

#### With contributions from:

Paulo J. Miranda da Silva Iwakami Beltrão, Sandra M. Naressi Scapin, Youssef Bacila Sade  
Instituto Nacional de Metrologia, Qualidade e Tecnologia (INMETRO)  
Xerém, Brazil

Adilah Bahadoor, Bradley B. Stocks, Marie-Pier Thibeault, Jeremy E. Melanson  
Measurement Science and Standards - National Research Council of Canada (NRC)  
Ottawa, Canada

Chiara Giangrande, Vincent Delatour, Amandine Boeuf, H el ene Vaneeckhoutte  
Laboratoire National de M etrologie et d'Essais (LNE)  
Paris, France

R udiger Ohlendorf, Gavin O'Connor, Andre Henrion  
Physikalisch-Technische Bundesanstalt (PTB)  
Braunschweig, Germany

Wai-Hong Fung, Yiu-Tung Wong  
Government Laboratory (GLHK)  
Kowloon, Hong Kong, China

Kazumi Saikusa, Taichi Yamasaki, Tomoya Kinumi  
National Metrology Institute of Japan (NMIJ), National Institute of Advanced Industrial Science  
and Technology (AIST)  
Tsukuba, Japan

Merve Oztug, Evren Saban, M usl um Akg oz  
National Metrology Institute of Turkey (TUBITAK UME)  
Gebze-Kocaeli, Turkey

Milena Quaglia, Kate Groves, Cailean Clarkson, Giles Drinkwater, David Rup erez Cebolla  
LGC Limited (LGC)  
Teddington, United Kingdom

**Coordinating laboratory contact:** Ralf D. Josephs ([ralf.josephs@bipm.org](mailto:ralf.josephs@bipm.org))

## **TABLE OF CONTENT**

INTRODUCTION

RATIONALE/PURPOSE

CHARACTERIZATION OF STUDY MATERIAL

CHARACTERIZATION STUDIES

HOMOGENEITY STUDIES

STABILITY STUDIES

SORPTION MEASUREMENTS

SAMPLE DISTRIBUTION

QUANTITIES AND UNITS

### **REPORTED MASS FRACTIONS OF VE AND IMPURITIES IN CCQM-K115.2018**

- Peptide Related Impurity Profile of CCQM-K115.2018

KEY COMPARISON REFERENCE VALUES (KCRVS) FOR CCQM-K115.2018

- Impurity Profile and Key Comparison Reference Value (KCRV) for the Mass Fraction of Peptide Related Impurities in CCQM-K115.2018
- Key Comparison Reference Value (KCRV) for the Mass Fraction of VE in CCQM-K115.2018

CONCLUSIONS

HOW FAR THE LIGHT SHINES STATEMENT (HFTLS)

ACKNOWLEDGEMENTS

REFERENCES

## INTRODUCTION

Comparability of (bio)chemical measurements is a prerequisite of any measurement undertaken in support of legislative purposes. For most chemical analysis this can be achieved by ensuring that measurement results are traceable to a known reference such as the base units of the *Système International d'Unités* (SI) [1]. By maintaining such a link, results can be compared over time and space enabling informed decisions to be made and improving our overall knowledge of a subject area. The importance of traceable measurement results can be inferred by its requirement in quality standards (ISO 17025) and in the formation of specialized committees as the Joint Committee on Traceability in Laboratory Medicine (JCTLM). However, whilst the required metrological tools, such as higher order reference measurements procedures, pure substance and matrix certified reference materials, are established for small well defined molecules difficulties still remain in the provision of such standards in the area of larger biomolecules notably peptides/proteins.

The provision of Primary Calibration Reference Services has been identified as a core technical competency for National Metrology Institutes (NMIs) and Designated Institutes (DIs) [2]. NMIs/DIs providing measurement services in peptide/protein analysis are expected to participate in a limited number of comparisons that are intended to test and demonstrate their capabilities in this area.

Primary Calibration Reference Services refers to a technical capability for composition assignment, usually as the mass fraction content, of a peptide/protein in the form of high purity solids or standard solutions thereof.

The assignment of the mass fraction content of high purity materials is the subject of the CCQM-K115 comparison series. A model to classify peptides in terms of their, relative molecular mass, the amount of cross-linking, and modifications has been developed and upgraded as it is depicted in Figure 1 [1,3]. With the aim of leveraging the work required for the CCQM-K115 comparison and thereby minimising the workload for NMIs/DIs and simultaneously focussing on a material directly relevant to existing CMC claims, human C-peptide (hCP) was the most appropriate choice for a study material for a first CCQM key comparison and parallel pilot study looking at competencies to perform peptide purity mass fraction assignment. hCP covers the space of quadrant A of the model as it allowed generic capabilities to be demonstrated for linear peptides without cross-links and of up to 31 amino acids in length [4,5]. The second cycle of peptide purity comparisons, CCQM-K115.b/P55.2.b on oxytocin (OXT) covered the space of quadrant A for short (1 kDa to 5 kDa), cross-linked and non-modified synthetic peptides as OXT is a cyclic peptide possessing nine amino acid residues and a disulfide bond. OXT is a chemically synthesized peptide hormone [6,7].

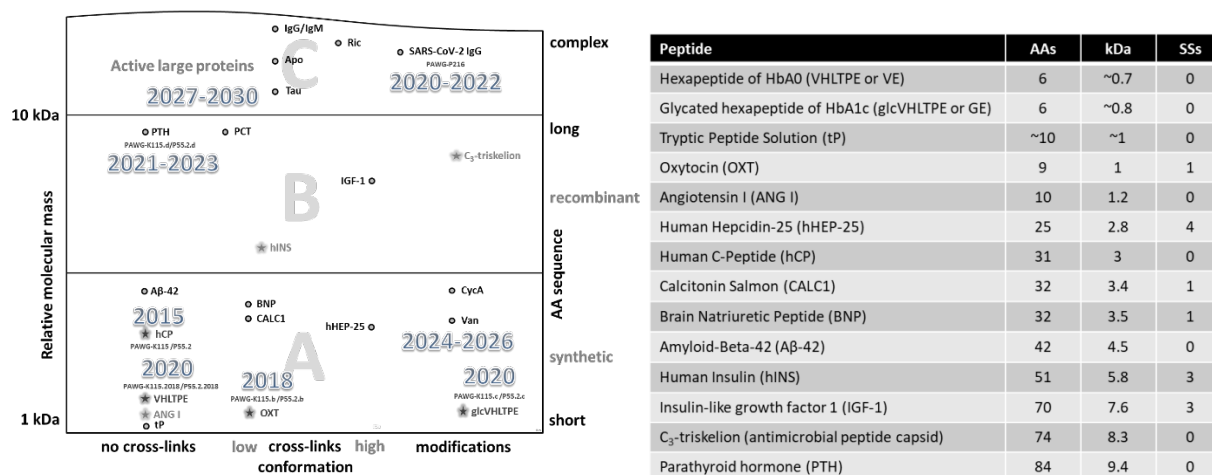


Figure 1: Model for the classification of peptides for primary structure purity determinations

## RATIONALE/PURPOSE

The approach taken for small molecules relies on Primary Calibrators, often in the form of a synthetic standard of known purity. The provision of Primary Calibration Reference Services has been identified as a core technical competency for NMIs/DIs in the strategy developed for the planning of ongoing Key Comparisons of the Organic Analysis Working Group (OAWG) within the Comité Consultatif pour la Quantité de Matière (CCQM) [8]. NMIs/DIs providing measurement services in organic analysis are expected to participate in a limited number of Track A comparisons that are intended to test and demonstrate their capabilities in this area. Primary Calibration Reference Services refers to a technical capability for composition assignment, usually as the mass fraction content, of organic compound(s) such as pure substances or solutions. The procedure adopted by most NMIs/DIs, for the provision of primary pure substance calibrators relies on a mass balance approach. This can be determined either by approaches that measure the mass fraction or mole fraction of the main component directly, or by indirect approaches that identify and estimate the mass fraction of the individual impurities and/or distinct classes of impurities present in the material and, by subtraction, provide a measure for the main component of the material [9]. These approaches have been successfully applied to a large variety of small molecules [10-14].

The quantification of larger molecules is complicated by the fact that they can exhibit higher order structures, and that characterization of the primary structure of the molecule maybe insufficient to correlate the amount of the molecule to its biological activity. Nevertheless, the quantification of the primary structure purity of a larger molecule is the first step in establishing a primary calibrator material for that molecule, where the quantity of interest is the mass fraction of the large molecule. The current discussion is limited to the measurement of the primary structure mass fraction of the molecule within a material.

Another complication for the provision of traceable peptide/protein measurements is that pure peptides/proteins can usually not be obtained in sufficiently large quantities. This has resulted in the harmonisation of many large molecule measurements by the provision of accepted practices, methods and/or standards. However, the increased use of targeted hydrolysis based digestion and peptide quantification strategies has enabled the determination of protein amounts via prototypic peptides [15-17]. These approaches have been investigated for example for the routine analysis of human growth hormone and its biomarkers [18-19]. A number of NMIs/DIs have been developing higher order measurement procedures for the analysis of purified protein calibrators [20] and serum based matrix materials [19]. These approaches show great promise for the standardisation of priority protein measurands. However, the mass fraction value assignment of proteins requires proteotypic peptides of known purity [1].

The purity of proteotypic peptides and peptides that show direct bioactivity by themselves can be assessed by use of the full mass balance approach. However, a full mass balance approach could require unviably large quantities of peptide material. A simpler alternative to the full mass balance approach is a peptide impurity corrected amino acid (PICAA) analysis, requiring quantification of constituent amino acids following hydrolysis of the material and correction for amino acids originating from impurities [4-7, 21-22]. It requires identification and quantification of peptide impurities for the most accurate results.

Traceability of the amino acid analysis results is to pure amino acid certified reference materials (CRMs). Few pure amino acid CRMs are commercially available. Alternatively, traceability could be established through in-house or NMI purity capabilities for amino acids. NMI capabilities to determine the purity of L-valine, were assessed in the CCQM-K55.c comparison in the frame of the OAWG [12]. In addition, amino acid analysis and peptide hydrolysis capabilities for the mass concentration assignment of peptide solutions are evaluated in the series of CCQM-P55 comparisons in the framework of the former BAWG using peptide materials of unknown purity [1].

The application of other approaches for the assessment of peptide purity that require only minor quantities of peptide material is conceivable, for example elemental analysis (CHN/O) with a correction for nitrogen originating from impurities or quantitative nuclear magnetic resonance (qNMR) spectroscopy with a correction for structurally-related peptide impurities (PICqNMR) [1, 4, 23].

The present CCQM-K115.2018 study 'Key Comparison Study on Peptide Purity - Hexapeptide of HbA0' (VE) is the first repeated study of the CCQM-K115 series to cover the space of quadrant A of the model as it allowed generic capabilities to be demonstrated for linear peptides without cross-links and of up to 5 kDa. The timeline for the CCQM-K115.2018 key comparison on VE is summarized in Table 1.

Table 1: CCQM-K115.2018 Timetable

Action	Date
Initial discussion	October 2016 and April 2017 PAWG meetings
Approval of Study Proposal	September 2017 PAWG meeting
Draft protocol and confirmation	April 2018 PAWG meeting
Sample characterization completed	January 2019
Call for participation	April 1 <sup>st</sup> , 2019
Final date to register	April 30 <sup>th</sup> , 2019
Sample distribution	June to July 2019
Date due to coordinator	September 18 <sup>th</sup> , 2020
Justification for 14 months period	Shifted several times because of the coronavirus pandemic
Initial report and discussion of results	November 2020 PAWG meeting
Discussion and reference value established	April 2021 PAWG meeting
Draft B report	March 2022 approved by PAWG
Final report to PAWG Chair	July 2022

## CHARACTERIZATION OF STUDY MATERIAL

The mass fraction of the hexapeptide of HbA0 (VE) in the material is to be determined. VE is defined as hemoglobin subunit beta [2-7] fragment with the amino acid sequence VHLTPE and a relative molecular mass ( $M_r$ ) of about 694.7 g/mol.

The study material was prepared by the BIPM/HSA by characterization of a commercially sourced sample of synthetic VE. The methods used to investigate, assign and confirm the quantitative composition of the CCQM-K115.2018 and CCQM-P55.2.2018 candidate material by the BIPM are summarized below.

## CHARACTERIZATION STUDIES

Peptide related impurity content was evaluated by

- LC-hrMS/MS

Water content was evaluated by

- Coulometric Karl Fischer titration (KFT) with oven transfer of water from the sample
- Thermogravimetric analysis (TGA) as a consistency check for the assigned value
- Microanalysis (% C, H, N content) as a consistency check for assigned value
- Sorption balance measurements

Residual solvent content was evaluated by

- GC-MS by direct injection
- <sup>1</sup>H-NMR
- Thermogravimetric analysis as a consistency check for the assigned value
- Microanalysis (% C, H, N content) as a consistency check for the assigned value

Non-volatile/ inorganics content by

- <sup>19</sup>F-NMR
- IC for common elements and counter ions (acetate, chloride, formate, nitrate, oxalate, phosphate, sulfate, trifluoroacetate (TFA), ammonium, calcium, magnesium, potassium, sodium) as a consistency check for the assigned values
- Microanalysis (% C, H, N content) as a consistency check for the assigned values

The BIPM/HSA have

- investigated the levels of within and between vial homogeneity of the main component and selected significant minor components;
- identified a minimum sample size which reduces to an acceptable level the effect of between-bottle inhomogeneity of both the main component and the minor components;
- completed isochronous stability studies of both the main component and the minor components to confirm that the material is sufficiently stable within the proposed time scale of the study if stored at low temperature (4 °C to -20 °C);
- determined appropriate conditions for its storage (4 °C to -20 °C), transport (cooled and temperature controlled) and handling;
- studied the impact of the relative humidity and temperature on the water content and provide a correction function for the gravimetric preparation of the comparison sample.



## HOMOGENEITY STUDIES

The BIPM/HSA have investigated the levels of within and between vial homogeneity of the main component and selected significant minor components and have identified a minimum sample size which reduces to an acceptable level the effect of between bottle inhomogeneity of both the main component and the minor components [24].

The results of the ANOVA are summarised in Table 2. No differences in the within- and between-sample variances could be detected by the F-tests at the 95 % confidence level. The material could be regarded as homogeneous. For methylated VE (VE+Me) and alanine inserted VE (VE+A), the  $s_{bb}$  could not be calculated due to the fact that for all  $MS_{\text{between}}$  was smaller than  $MS_{\text{within}}$ . The  $u^*_{bb}$  of 1.77 %, 0.95 %, and 1.41 % was adopted as an estimate for the uncertainty contribution due to potential inhomogeneity for VE, methylated VE (VE+Me) and alanine inserted VE (VE+A). The impurities VE+Me and VE+A represent high (about 1.6 mg/g) and low (about 0.6 mg/g) mass fractions level impurities, respectively.

Table 2: Homogeneity results of representative VE and selected VE impurities

	VE	VE+Me High level	VE+A Low level
N	29	29	29
$s_{wb}$ (%)	4.08	2.94	4.33
$s_{bb}$ (%)	1.77	-( <sup>1</sup> )	-( <sup>1</sup> )
$u^*_{bb}$ (%)	1.33	0.95	1.41
$u_{bb}^{(2)}$ (%)	<b>1.77</b>	<b>0.95</b>	<b>1.41</b>
F	1.562	0.859	0.786
$F_{\text{crit}}$	2.393	2.393	2.393

(<sup>1</sup>) Not calculable because  $MS_{\text{between}} < MS_{\text{within}}$

(<sup>2</sup>) Higher value ( $u^*_{bb}$  or  $s_{bb}$ ) was taken as uncertainty estimate for potential inhomogeneity

Linear regression functions were calculated for the results according to analysis order. The slopes of the lines were tested for significance on a 95 % confidence level to check for significant trends. No significant trend was observed for the injection sequences. The normalized result due to the analysis and filling sequences are presented in the Figures 2-4. The first, second and third replicates are represented by circles, grey filled circles and dots respectively.

The homogeneity of the pure CCQM-K115.2018 VE candidate material was studied using an LC-UV-hrMS method for the quantitative determination of VE, methylated VE (VE+Me) and alanine inserted VE (VE+A). Acceptable uncertainties due to inhomogeneity were obtained for the pure VE material by use of the LC-hrMS method under repeatability conditions applying mass spectrometric detection for the main component and inherent related impurities. Absolute uncertainties due to between unit inhomogeneity of 0.015 mg/g (0.95 %) and 0.008 mg/g (1.41 %) could be assigned to the inherent impurities of VE+Me and VE+A, respectively. In addition, an uncertainty contribution due to between unit inhomogeneity ( $u_{bb}$ ) of 11.1 mg/g (1.77 %) for the

VE content was verified by use of UV detection. Therefore, this candidate material is appropriate to serve in the CCQM-K115.2018 study to evaluate mass fraction range of inherent impurities, provided a suitable sample intake of more than 2.5 mg is used for analysis of the material.

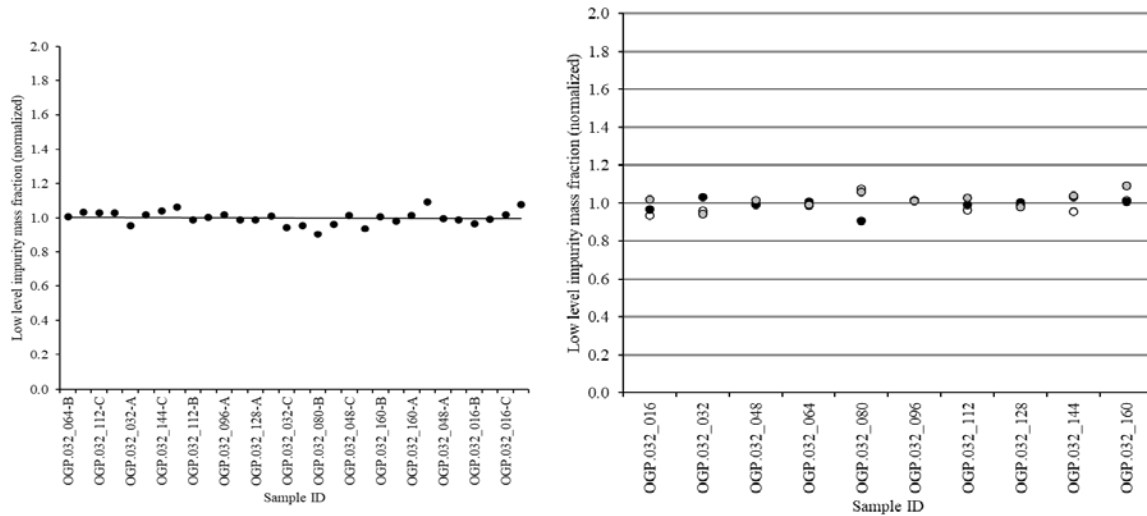


Figure 2: Homogeneity of VE+A - Low level mass fraction impurity - Injection and filling sequence

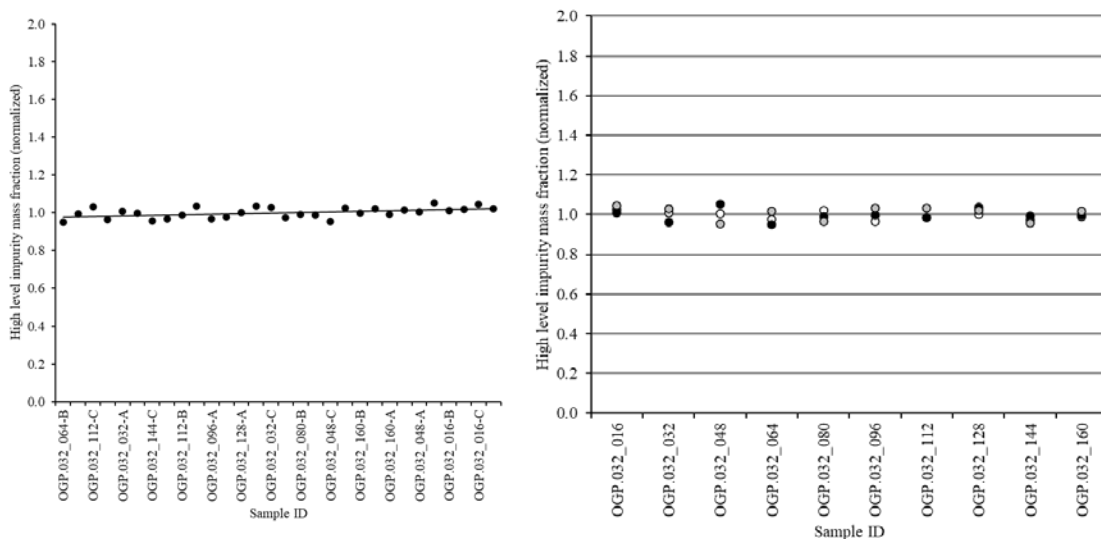


Figure 3: Homogeneity of VE+Me - High level mass fraction impurity - Injection and filling sequence

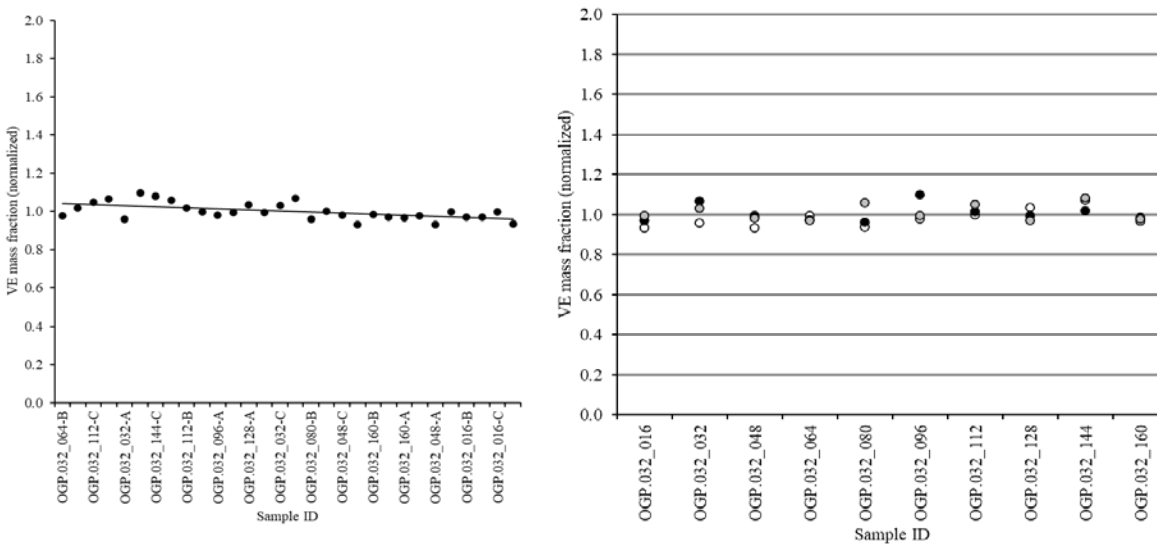


Figure 4: Homogeneity of VE - Injection and filling sequence

## STABILITY STUDIES

Isochronous stability studies were performed using a reference storage temperature of  $-20\text{ }^{\circ}\text{C}$  and test temperatures of  $4\text{ }^{\circ}\text{C}$ ,  $22\text{ }^{\circ}\text{C}$  and  $40\text{ }^{\circ}\text{C}$ . A set of units from the production batch were stored at each selected temperature over 8 weeks, with units transferred to reference temperature storage at 2 week intervals.

Trend analysis of the data obtained by LC-UV-hrMS analysis of the stability test samples under repeatability conditions indicated no significant changes in the relative composition of VE or of the related peptide impurities over longer time and at low temperatures.

The VE mass fraction of the material was stable on storage at  $4\text{ }^{\circ}\text{C}$ ,  $22\text{ }^{\circ}\text{C}$  and  $40\text{ }^{\circ}\text{C}$  over the entire storage study period. The VE+Me mass fraction of the material, representing high mass fraction level impurities, was stable on storage but did decrease significantly after storage beyond 2 weeks at  $4\text{ }^{\circ}\text{C}$ . The VE+Me mass fraction did decrease significantly over the entire storage study period at both  $22\text{ }^{\circ}\text{C}$  and  $40\text{ }^{\circ}\text{C}$ . The peptide related impurity VE+A mass fraction of the material, representing low mass fraction level impurities, was stable on storage at  $4\text{ }^{\circ}\text{C}$  over the entire storage study period and did increase significantly and slightly after storage beyond 4 weeks at  $22\text{ }^{\circ}\text{C}$ . The peptide related impurity VE+A mass fraction of the material did not change significantly after storage beyond 4 weeks at  $40\text{ }^{\circ}\text{C}$ .

The effect of storage temperatures on the mass fractions of VE and related peptide impurities of the comparison material is shown in Figures 5-7.

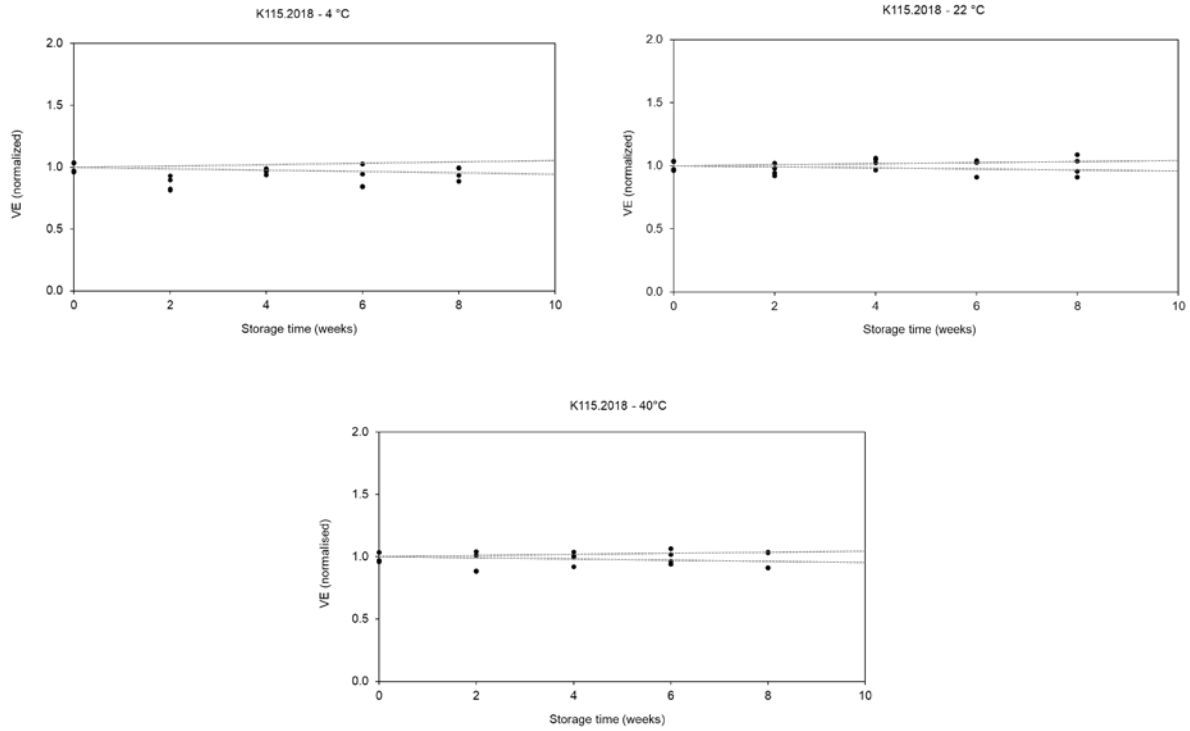


Figure 5: Stability study of VE

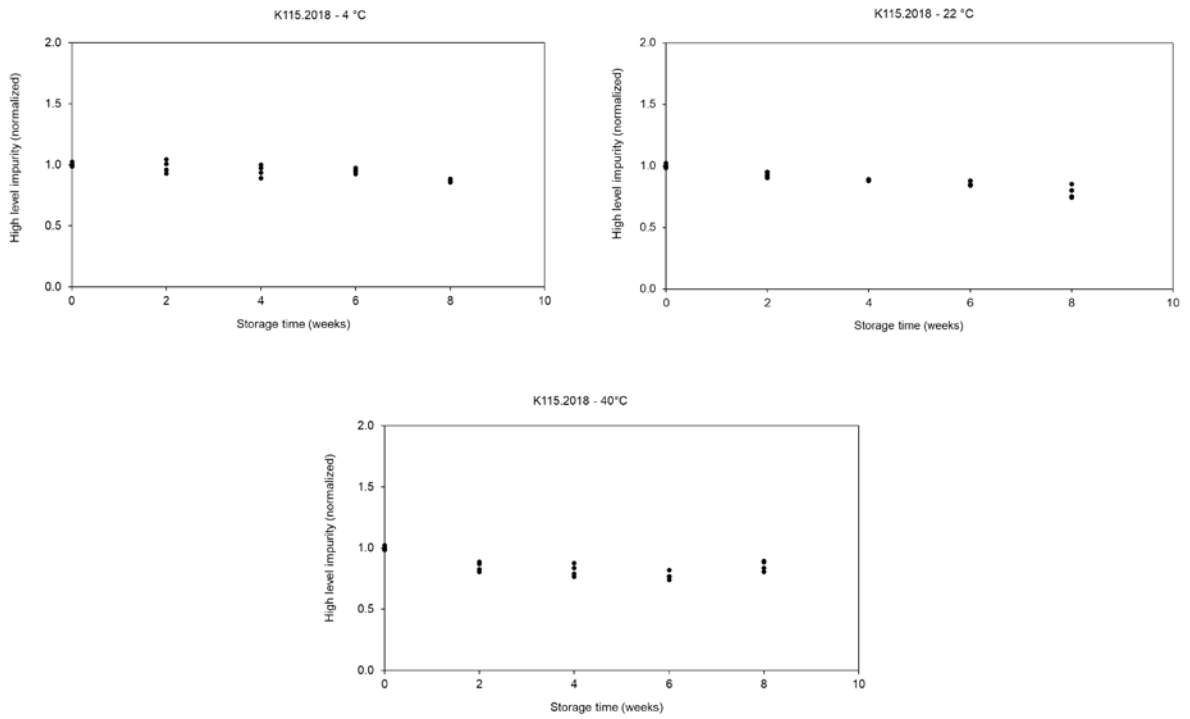


Figure 6: Stability study of VE+Me - High level mass fraction impurity

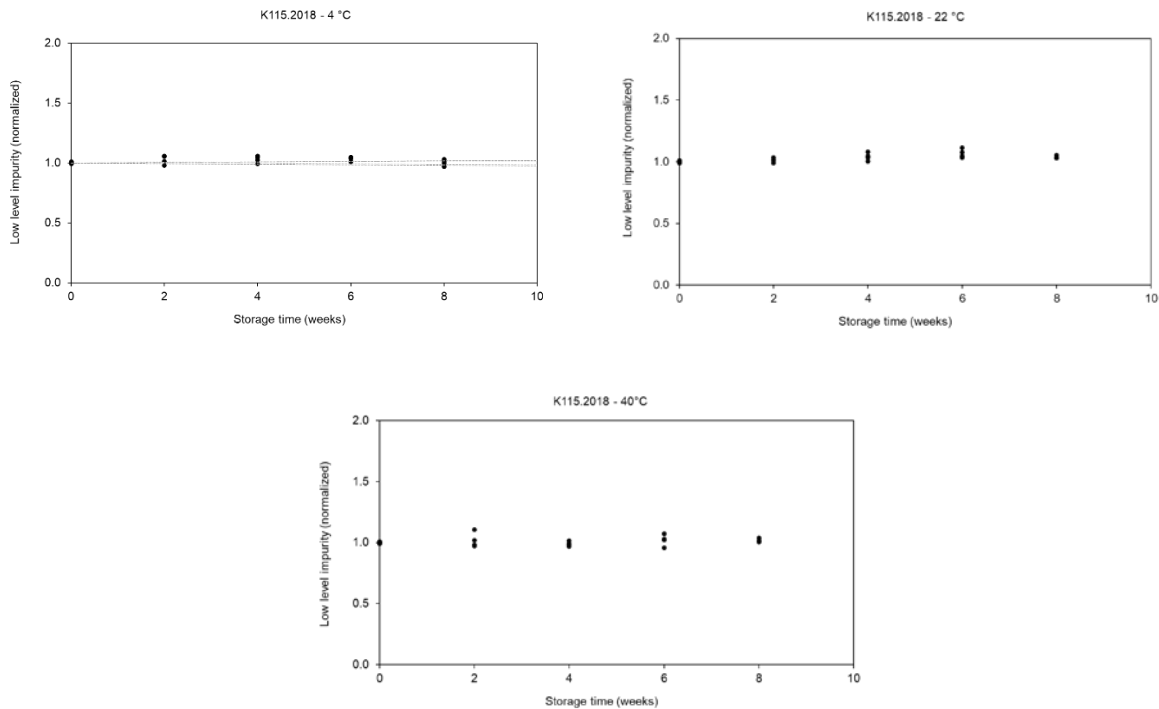


Figure 7: Stability study of VE+A - Low level mass fraction impurity

On the basis of these studies, it was concluded that for the purposes of the comparison the material was suitably stable for short-term cooled transport at low temperatures, provided it was not exposed to temperatures significantly in excess of 4 °C for more than 2 weeks, and for longer term storage at -20 °C.

The vials were shipped by courier using insulated shipping containers under -20 °C. The internal temperatures were recorded by data loggers.

To minimize the potential for changes in the material composition, participants were instructed to store the material in the freezer at -20 °C.

**SORPTION MEASUREMENTS**

Additional measurements performed on a dynamic vapor sorption (DVS) balance indicate that weighings of the CCQM-K115.2018 comparison material need to be performed under controlled conditions of temperature and relative humidity (RH) as the water content of the comparison material changes reversibly as a function of the RH (Figure 8).

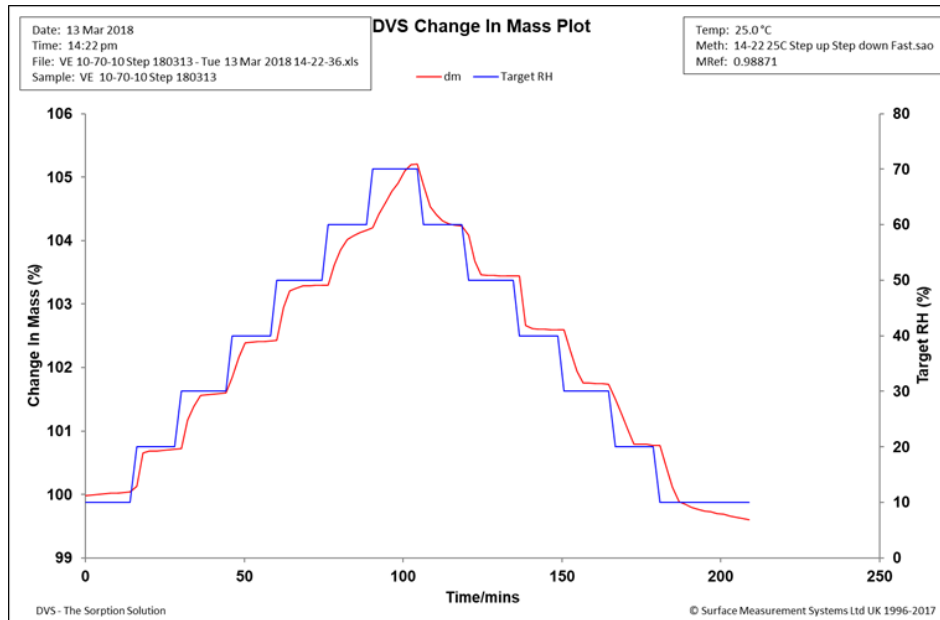


Figure 8: Sorption balance measurements indicating reversible water adsorption/desorption. Influence of RH (blue, % RH) on relative mass of VE (red, % change).

The temperature at which weighings are performed had to be measured and reported and had to be maintained between 20 °C and 30 °C. The relative humidity (RH<sub>X</sub>) at which weightings of the powdered material were performed has been recorded. The RH range over which the material can be weighed is between 30 % and 70 %. After opening of the vial, the comparison material needs to equilibrate at constant RH<sub>X</sub> for a minimum of 60 min before starting the weighing process. The mass of sample (M<sub>RHX</sub>) measured at the relative humidity (RH<sub>X</sub>) shall be corrected to the mass of sample (M<sub>RH50</sub>) at a RH of 50 % using the numerical equation:

$$M_{RH50} = M_{RHX} / (1 + F \cdot (RHX - 50))$$

where  $F = 0.0008$  and  $u(F) = 0.0001$

RHX is the numerical value of the measured relative humidity expressed in %.

(Note: Relative humidity measurements with a standard uncertainty of 2 % and temperature measurements with a standard uncertainty of 0.2 °C will be sufficient to achieve the required accuracy for this correction)

## **SAMPLE DISTRIBUTION**

Samples were distributed by HSA to all participants and the co-coordinating institutes (BIPM and NIM) in June and July 2019.

Two units of the study sample, each containing a minimum of 25 mg of materials, were distributed to each participant by express mail service in insulated and cooled transport containers equipped with a temperature data logger to record the temperature throughout the transport process. Participants were asked to return the sample receipt form and the data logger report acknowledging receipt of the samples and to advise the coordinators if any obvious damage had occurred during the shipping. All participants except INMETRO received the samples within one week from the time the samples were shipped out. The data logger reports to all participants except NRC and TUBITAK UME showed that the samples had not been exposed to temperature above 8 °C during the transport process. The data logger reports to NRC and TUBITAK UME showed that the samples had been exposed to temperature above 8 °C for about one day (highest temperature reached: 15.3 °C for samples to NRC and 13.2 °C for samples to TUBITAK UME). As the time above 8 °C was very short and the temperature did not even reach room temperature, the coordinators concluded that the samples were still appropriate for study. The samples to INMETRO were held at Brazilian custom for very long time and were finally destroyed. INMETRO arranged a subcontractor to collect the replacement samples in January 2020.

As co-coordinating institutes would use mass balance method to determine the purity of the material, 22 units of the study samples, each containing a minimum of 25 mg of material, were distributed to each co-coordinating institute (BIPM and NIM) in insulated and cooled transport containers. Temperature was monitored by the courier and ice pack top-up was requested to ensure the temperature to be maintained below 8 °C during the transport process. Both co-coordinating institutes received the samples within three days from the time the samples were shipped out.

## **QUANTITIES AND UNITS**

Participants were required to report the mass fraction of VE, the major component of the comparison sample. In addition, all participants who used a PICAA or qNMR procedure to determine the VE mass fraction were required to report the combined mass fraction assignment and corresponding uncertainty for total related peptide impurities.

In addition, the BIPM, HSA and NIM who employed a mass balance (summation of impurities) procedure to determine the VE mass fraction were required to report the combined mass fraction assignment and corresponding uncertainty for the sub-classes of total related peptide impurities, water, total residual organic solvent / volatile organic compounds (VOCs) and total non-volatile organics & inorganics.

Participants were encouraged to also provide mass fraction estimates for the main impurity components they identified in the comparison sample.

**REPORTED MASS FRACTIONS OF VE AND IMPURITIES IN CCQM-K115.2018**

The values reported by participants for the VE mass fraction in CCQM-K115.2018 are given in Table 3 with a summary plot in Figure 9. The values reported by participants for the peptide related impurity (PepImp) mass fractions in CCQM-K115.2018 are given in Table 6 with a summary plot in Figure 10.

The reported values for the VE mass fractions in CCQM-K115.2018 can be divided into two main groups - one group with both the BIPM and NIM using mass balance approaches and a second group using PICA approaches. NRC has used qNMR and HSA has reported the average of three approaches (mass fraction, PICA and IDMS).

Table 3: Results for CCQM-K115.2018: VE mass fractions and uncertainties as received

Participant	Mass fractions (mg/g)			Coverage Factor ( <i>k</i> )	Approach
	VE	<i>u</i> (VE)	<i>U</i> (VE)		
INMETRO, Brazil	626	22	44	2	PICAA
LNE, France	652.025	17.568	35.135	2	PICAA
NIM, China	679.5	5.0	10.1	2	Mass balance
BIPM	625.5	6.5	13.0	2	Mass balance
LGC, United Kingdom	593.5	3.6	11.4	3.2	PICAA/ PICqNMR
NMIJ, Japan	611.4	10.4	20.9	2	PICAA
NRC, Canada	630.3	10.1	20.2	2	PICqNMR
PTB, Germany	645.4	6.6	13.2	2	PICAA
UME, Turkey	603.8	17.8	35.5	2	PICAA
GLHK, Hong Kong	637	24.1	48.2	2	PICAA
HSA, Singapore	634.3	6.5	13.1	2	Mass balance/ PICAA/ IDMS



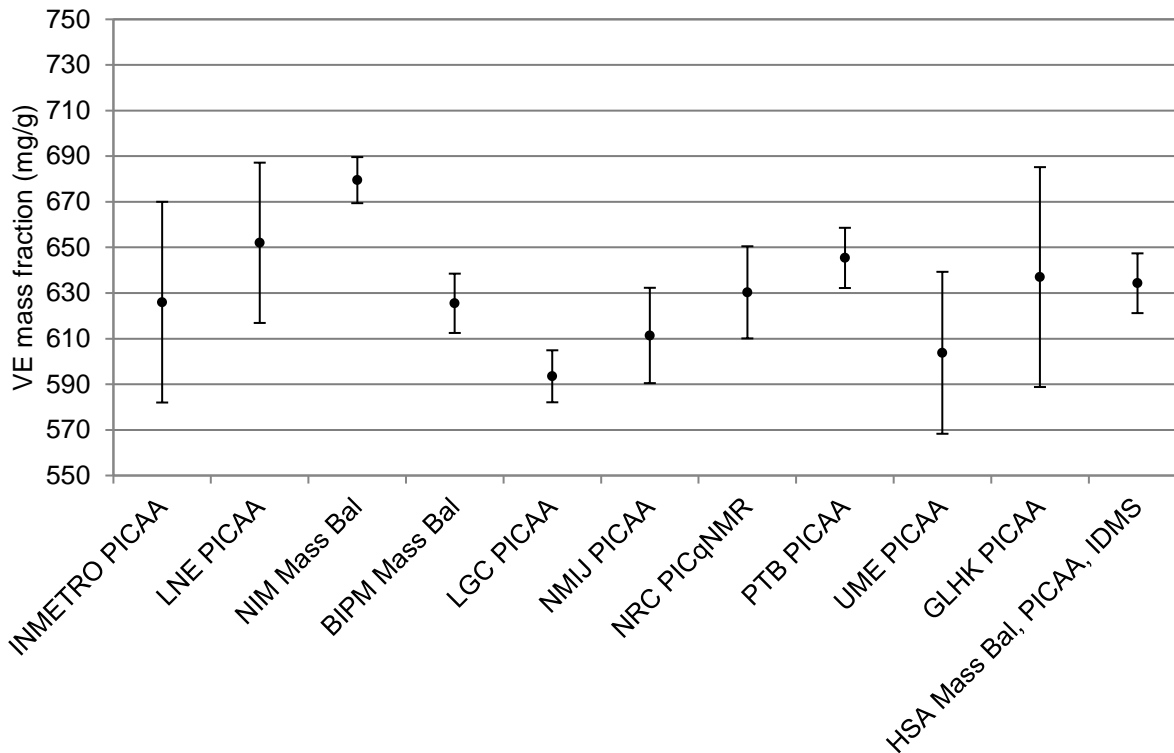


Figure 9: VE mass fractions reported by participants in CCQM-K115.2018 - plotted with expanded uncertainties ( $U$ ) at a confidence level of about 95 %

The VE mass fraction values obtained by the BIPM and NIM using a mass balance approach do not agree within their estimated uncertainties. The related peptide impurity profile obtained by BIPM and NIM are in agreement.

TFA impurity mass fraction values are listed in Table 4. TFA impurity mass fraction values obtained by  $^{19}\text{F}$ -qNMR were submitted by BIPM, HSA and NRC. In addition, both BIPM and NIM have submitted TFA impurity mass fraction values based by ion chromatography.  $^{19}\text{F}$ -qNMR TFA impurity mass fraction values obtained by HSA, NRC and BIPM are in agreement. The TFA impurity mass fraction value from NIM obtained by ion chromatography is significantly lower than the values obtained by  $^{19}\text{F}$ -qNMR. NIM has revised the ion chromatography mass fraction value after the PAWG meeting in April 2021 confirming issues with the TFA calibration CRM for ion chromatography. A revised NIM value is provided in brackets in Table 4 for information.

A total TFA mass fraction of 286.7 mg/g with a corresponding expanded uncertainty of 9.9 mg/g ( $k = 4.3$ ) could be calculated by use of the DerSimonian-Laird variance-weighted mean (DSL) [25-26] taking into consideration the TFA impurity mass fraction values obtained by  $^{19}\text{F}$ -qNMR. The DSL-mean takes into account the uncertainties while introducing sufficient excess variance to allow for their observed dispersion. The total TFA mass fraction is in agreement with the revised TFA impurity mass fraction value from NIM and the information value from BIPM both obtained by ion chromatography.

Water impurity mass fraction values obtained by KFT were submitted by BIPM, HSA, NIM and NRC (Table 5). Insufficient material was available for NRC to perform more than one measurement (i.e. no replicates) for the water content by KFT. The uncertainty listed by NRC is an estimate based on previous measurements and the value provided by NRC was not considered to calculate the total water mass fraction.

A total water mass fraction of about 47.5 mg/g with a corresponding expanded uncertainty of 17.6 mg/g ( $k = 4.3$ ) could be calculated by use of the DerSimonian-Laird variance-weighted mean (DSL) taking into consideration the water mass fraction values provided by HSA, NIM and BIPM obtained by KFT. All water impurity mass fraction values including the NRC value are in agreement.

Table 4: TFA mass fractions and uncertainties

Participant	Mass fractions (mg/g)			Coverage Factor ( $k$ )	Approach
	TFA	$u$ (TFA)	$U$ (TFA)		
HSA, Singapore	283.8	2.5	5.0	2	qNMR
NRC, Canada	282.4	7.8	15.6	2	qNMR
BIPM	289.0	0.8	1.5	2	qNMR
BIPM	295*	10*	20*	2*	IC*
NIM, China	254.2 (288.45)	4.6 (3.4)	9.1 (6.8)	2 (2)	IC (IC)

\* not traceable to the SI provided for information.


Table 5: Water mass fractions and uncertainties

Participant	Mass fractions (mg/g)			Coverage Factor ( $k$ )	Approach
	Water	$u$ (Water)	$U$ (Water)		
HSA, Singapore	48.17	4.61	9.22	2	KFT
BIPM	57.1	6.3	12.6	2	KFT
NIM, China	42.6	1.7	3.4	2	KFT
NRC, Canada	45	14	28	2	KFT

The peptide related impurities (PepImp) mass fractions values obtained by the participants in many cases agree within their estimated uncertainties. However, LGC, LNE and NRC have assigned a significantly higher values (Table 6). NRC was the only participant that clearly identified and quantified the one of the largest impurity VE depsipeptide as it becomes clear from NRCs individual components table that lists the *cis-trans* VE depsipeptide isomers as impurities.

Table 6: Results for CCQM-K115.2018: Overall peptide related impurities (PepImp) mass fractions and uncertainties as received

Participant	Mass fractions (mg/g)			Coverage Factor ( <i>k</i> )	Approach
	PepImp	<i>u</i> (PepImp)	<i>U</i> (PepImp)		
INMETRO, Brazil	27.2	5.4	15.1	2.8	LC-UV-hrMS
LNE, France	44.192	35.354	70.707	2	LC-hrMS
NIM, China	23	1.3	2.6	2	UHPLC-MS/MS and UHPLC-hrMS
BIPM	18.83	1.17	2.34	2	LC-hrMS
LGC, United Kingdom	54.6	3.0	6	2	UHPLC-MS/MS and UHPLC-hrMS
NMIJ, Japan	19.4	0.7	1.4	2	LC-hrMS
NRC, Canada	40.2	9.0	18	2	LC-hrMS and qNMR
PTB, Germany	12.8	0.55	1.1	2	LC-MS/MS
UME, Turkey	30	1.3	2.6	2	LC-MS/MS
GLHK, Hong Kong	24	3.44	6.88	2	LC-hrMS
HSA, Singapore	29.8	7.75	15.5	2	LC-UV and LC-MS/MS

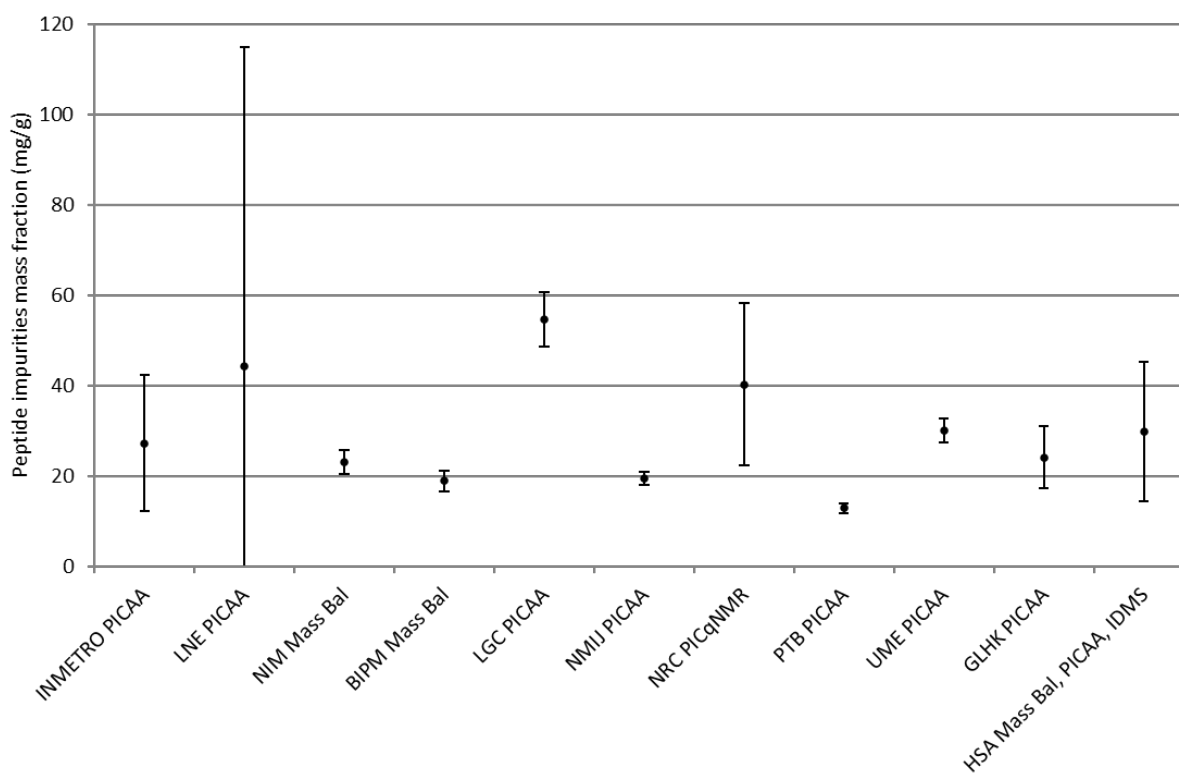Figure 10: Overall peptide related impurities (PepImp) mass fractions reported by participants in CCQM-K115.2018 - plotted with expanded uncertainties (*U*) at a confidence level of about 95 %

In general, the CCQM-K115.2018 and CCQM-P55.2.2018 comparison on VE purity shows less agreement of participants' results as the previous CCQM-K115/CCQM-P55.2 series comparisons on hCP and OXT for peptide purity determinations. The peptide related impurity (PepImp) determinations showed a superior level of agreement as for hCP and inferior level of agreement as for OXT. However, there was discussion on possible reasons for the discrepancy between CCQM-K115.2018/CCQM-P55.2.2018 results after presentation of the results of participants at the PAWG meeting in November 2020 and April 2021.

The peptide related impurities identification and quantification (Figure 10) is still a weak point as for both comparison on hCP and OXT. The number of potential impurities is much smaller for VE compared with both hCP and OXT as VE exhibits a shorter primary sequence. All eleven laboratories have identified/quantified the larger peptide related impurity VE+Me resulting in mainly coherent estimations of the peptide related impurity mass fractions. However, the major peptide impurity, VE depsipeptide, has only been correctly identified and quantified by the NRC. Hence most of the other participants have underestimated the sum of peptide related impurity mass fractions. A few participants, for example BIPM, LGC, HSA and LNE, have observed an additional broad peak but it was not identified as VE depsipeptide. It has been discussed if that peak could relate to the VE depsipeptide if certain solvent conditions are maintained in LC-MS analysis as the VE depsipeptide is only stable at low pH conditions for a few days. The depsipeptide issue is discussed in detail in the section Peptide Related Impurity Profile of CCQM-K115.2018.

It has been pointed out that the use of synthesized impurity standards has a positive impact on the quantification of the peptide related impurity mass fractions. Four laboratories have used synthesized impurity standards to quantify major impurities. Seven participants have quantified the peptide related impurities using a response factor ( $RF = 1$ ), RF with correction factor or a relative response method although four participants have used synthesized impurity standards to a different degree. NIM used 13 synthesized impurity standards (purities taken into account), BIPM used 5 synthesized impurities standards (purities taken into account) to quantify the individual impurities and closely structurally related impurities. NMIJ and PTB have used 5 and 4 synthesized impurities standards, respectively, and have quantified others with  $RF = 1$ .

NIM and BIPM have used the mass balance approach in CCQM-K115.2018. HSA has used a combination of mass balance, PICAA and direct IDMS. NRC has used PICqNMR. LGC has used a combination of PICqNMR and PICAA. Six participants have used the PICAA approach. LGC has used microwave assisted hydrolysis. GLHK, HSA, INMETRO, LNE, NMIJ, PTB and UME have employed gas/liquid phase hydrolysis. However, all participants that have used PICAA have performed an efficiency correction for the hydrolysis methods. The peptide related impurities values have been broken down to establish a means to visualize identification and quantification issues for the peptide related impurities.

## Peptide Related Impurity Profile of CCQM-K115.2018

The BIPM has broken down the peptide related impurities values to establish a means to visualize identification and quantification issues for the peptide related impurities. Figure 12 shows more details on the peptide related impurities of the CCQM-K115.2018 or CCQM-P55.2.2018 studies. The graph shows the peptide impurities that have been identified, the mean of the corresponding mass fractions, the corresponding standard deviations and the corresponding number of laboratories that have identified and quantified that impurity. The maximum possible number of identifications is ten as there are ten theoretical independent data sets due to the fact that some laboratories have used the same peptide impurity data set twice for example to correct both PICA and PICqNMR results.

Please note that several laboratories have identified groups of impurities but the position of the modification was not or not entirely identified, for example VHLTPE(OMe).

In general, the identification and quantification of peptide impurities is quite coherent among laboratories. However, certain issues were discussed during the PAWG meetings in November 2020 and April 2021.

Three large peptide related impurities [1Ψ2, C(NH<sub>2</sub>)=N]VHLTPE (or equivalent impurities with a -0.98 mass shift related to VE as uniquely identifiable), VHLTPE(OMe) and VHLTPEE have been identified and quantified by ten out of eleven laboratories. However, the major peptide impurity, VE depsipeptide, has only been correctly identified and quantified by the NRC via <sup>1</sup>H-NMR. The structures of peptides containing β-hydroxy amino acids, i.e. serine and threonine can alter as a result of an N- to O- acyl shift. In the process the amide linkage of the peptide backbone due to the component is cleaved and replaced by an ester bond at the β-hydroxyl group. In the case of the VE peptide, N- to O- acyl shift can potentially occur at the leucine-threonine junction via a stable five-membered ring cyclic intermediate as exemplarily depicted for the non-glycated hexapeptide (VE) in Figure 11. The formed VE depsipeptide exists as a mixture of *cis-trans* isomers in solution [27-29].

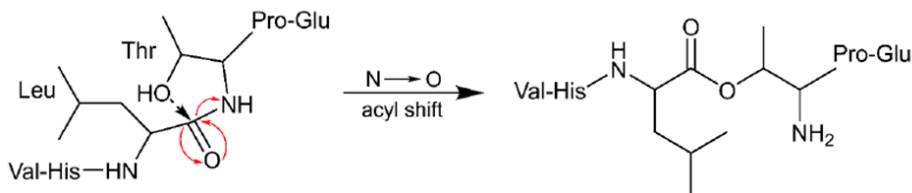


Figure 11: N to O acyl shift exemplarily depicted for non-glycated hexapeptide (VE)

The NRC has identified and quantified both *cis*- and *trans*-isomers of the VE depsipeptide via <sup>1</sup>H-NMR at mass fraction levels of  $5.9 \pm 3.6$  mg/g ( $k = 2$ ) and  $14.2 \pm 8.6$  mg/g ( $k = 2$ ), respectively. Related peptide impurities of that large mass fraction levels should have been identified and

quantified by other participants using  $^1\text{H-NMR}$ . The BIPM has agreed during the PAWG meeting in November 2020 to re-assess their own data concerning the presence of VE depsipeptide impurity fragments. In summary, the 2D COSY spectrum obtained on a VE sample in  $\text{D}_2\text{O}$  was re-analyzed and the VE depsipeptide isomers were identified. Given that the quantification signals were based on histidine protons, the purity values should have been corrected for the amount of depsipeptides. The approximate depsipeptide mass fractions were calculated in the VE samples in deuteromethanol. The combined VE depsipeptide mass fraction was  $15.2 \pm 0.4$  mg/g based on the integration of the signal due to the threonine  $\gamma\text{-CH}_3$  protons. The VE depsipeptide mass fraction assignments of the BIPM are in agreement and confirming the findings of the NRC.

The identification and quantification of the VE depsipeptide by use of LC-(hr)MS(/MS) techniques have proved to be difficult. Initially, the VE depsipeptide impurity was missed or misinterpreted by all participants using by LC-(hr)MS(/MS). Several participants, notably the BIPM, LGC and LNE, have observed a very broad peak eluting at shorter retention times than the main VE peak but it was not identified as VE depsipeptide. The BIPM and HSA have agreed during the PAWG meeting in November 2020 to re-assess their LC-(hr)MS data. Retrospective analysis of mass spectrometry data and subsequent investigations led to the conclusion that the presence of the VE depsipeptide was wrongly ignored. A VE isomer eluting before the main VE peak was quantified but eventually disqualified as an artefact because of inconsistent abundance in VE samples. The MS spectra showed that the broad peak was isobaric with VE but presented some characteristic water loss ions. The inconsistent peak area assignments could be attributed to the instability of depsipeptides and its pH dependency, as evidenced in subsequent experiments performed. It was confirmed that the VE depsipeptide is only present in freshly prepared aqueous solution of the VE material. Aqueous solutions are acidic (about pH 4) due to the high TFA content of the VE material. The VE depsipeptide peak decreased and disappeared completely after a few days (< 4 days) when the VE sample is prepared in an acidic aqueous solution (pH 4). The VE depsipeptide peak disappeared instantly when VE materials were dissolved in alkaline buffer (pH 9). The HSA investigated HPLC behavior of the VE depsipeptide using pure VE depsipeptide standard material. It was found that when pH ~ 6.0 mobile phase (20 mM ammonium acetate) was used, VE depsipeptide appeared as a broad peak right after VE peak. The same broad peak was observed in the comparison sample, which confirmed that VE depsipeptide had been accounted for as part of the total unknown impurities in HSA's report. It was also found that when pH ~2.8 mobile phase (0.1 % formic acid) was used, VE depsipeptide appeared as a broad peak at a shorter retention time than the VE peak, which was consistent with what was observed by BIPM, LGC and LNE. In addition, HSA also proved that the VE depsipeptide transformation in alkaline or weak acid solution (pH > 4) is irreversible (no depsipeptide production upon re-acidification to pH ~ 2.5). These findings imply that the VE depsipeptide was already present in the solid material. It should be noted that the instability of depsipeptide impurities could impact measurements for clinical purposes if the LC-MS methods used are employed under alkaline conditions.

Furthermore, it has been decided during the discussions within the CCQM PAWG in April 2021 that the VE depsipeptide structural isomer would be counted as impurity whereas the stereoisomers *cis/trans*, also present in the material, would not be counted as separate impurities.

UME has also re-assessed their data and in retrospect reported a quantification mismatch (0.45 mg/g instead of 9.12 mg/g) for Ac-HLTPE.

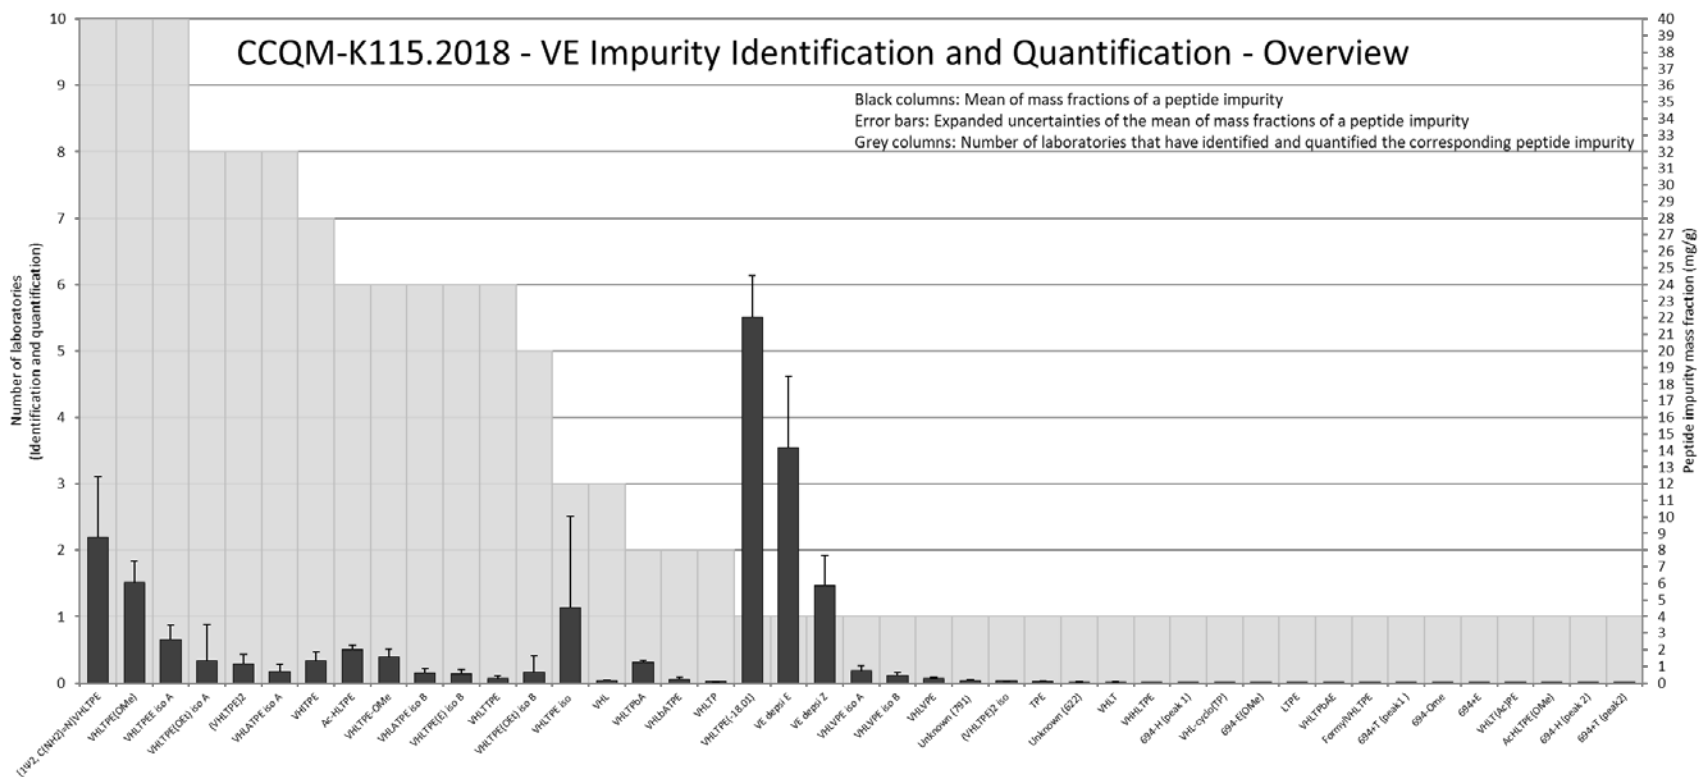


Figure 12: VE impurity identification and quantification - Overview



## KEY COMPARISON REFERENCE VALUES (KCRVS) FOR CCQM-K115.2018

The values used to establish the Key Comparison Reference Values (KCRV) for CCQM-K115.2018 are summarized in Table 3 and Table 6 for the VE mass fraction and the peptide related impurity mass fractions, respectively. All participants in CCQM-K115.2018 were required to give estimates for the mass fraction of the sub-class of peptide related impurities they quantified to obtain their final VE mass fraction estimate. The coordinator has calculated the overall KCRV for VE mass fraction and separate KCRV for the peptide related impurities as the peptide related impurity profile and quantification is of utmost importance.

### Impurity Profile and Key Comparison Reference Value (KCRV) for Mass Fraction of Peptide Related Impurities in CCQM-K115.2018

The  $KCRV_{PepImp}$  for the mass fraction of peptide impurities is based on the assumption that only the most consistent set of results is taken for the calculation of the  $KCRV_{PepImp}$ . The sum of the combined *cis/trans* VE depsipeptide impurities (only identified/quantified by NRC and confirmed by BIPM and HSA) and the means of the mass fractions of peptide related impurities that have been identified by at least two participants according to Figure 12 (impurities starting on the left until VHTLP inclusive) have been used to establish the  $KCRV_{PepImp}$ . The corresponding standard uncertainty ( $u(KCRV_{PepImp})$ ) of the  $KCRV_{PepImp}$  is the combined uncertainty of the individual uncertainties provided by the participants for the individual peptide impurities that have been considered. Peptide related impurities that have not been confirmed by at least one other participant are not considered.

Figure 13 shows the participant results with their reported standard uncertainties plotted against the  $KCRV_{PepImp}$  of 53.0 mg/g for peptide impurities in CCQM-K115.2018 (solid line) and its corresponding standard uncertainty of 8.6 mg/g ( $k = 1$ ). A corresponding expanded uncertainty of 17.3 mg/g ( $k = 2$ ) at a confidence level of about 95 % was calculated.

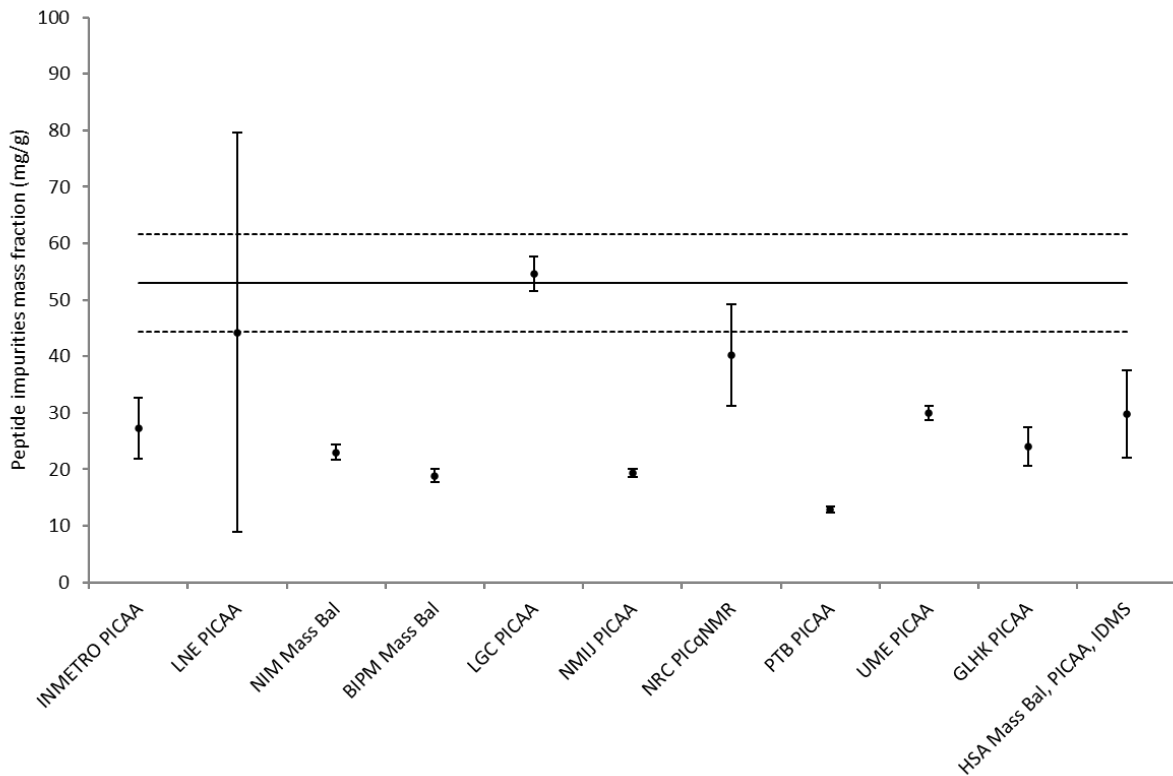


Figure 13: Estimates of total related peptide impurities in CCQM-K115.2018 plotted with their reported standard uncertainties ( $\pm u_c$ ,  $k = 1$ ). The  $KCRV_{PepImp}$  (solid line) is 53.0 mg/g. Dashed lines show the  $u(KCRV_{PepImp})$  ( $k = 1$ ) of the  $KCRV_{PepImp}$ .

The degree of equivalence of a participant's result with the  $KCRV_{PepImp}$  ( $D_i$ ) is given by:

$$D_i = w_i - KCRV_{PepImp}$$

The expanded uncertainty  $U_i$  at a confidence level of about 95 % associated with the  $D_i$  was calculated as [30]:

$$U_{95\%}(D_i) = 2 \cdot \sqrt{u(w_i)^2 + u(KCRV_{PepImp})^2}$$

Figure 14 indicates the degree of equivalence ( $D_i$ ) of each key comparison participant's result with the  $KCRV_{PepImp}$  for related peptide impurities. The corresponding values are listed in Table 7.

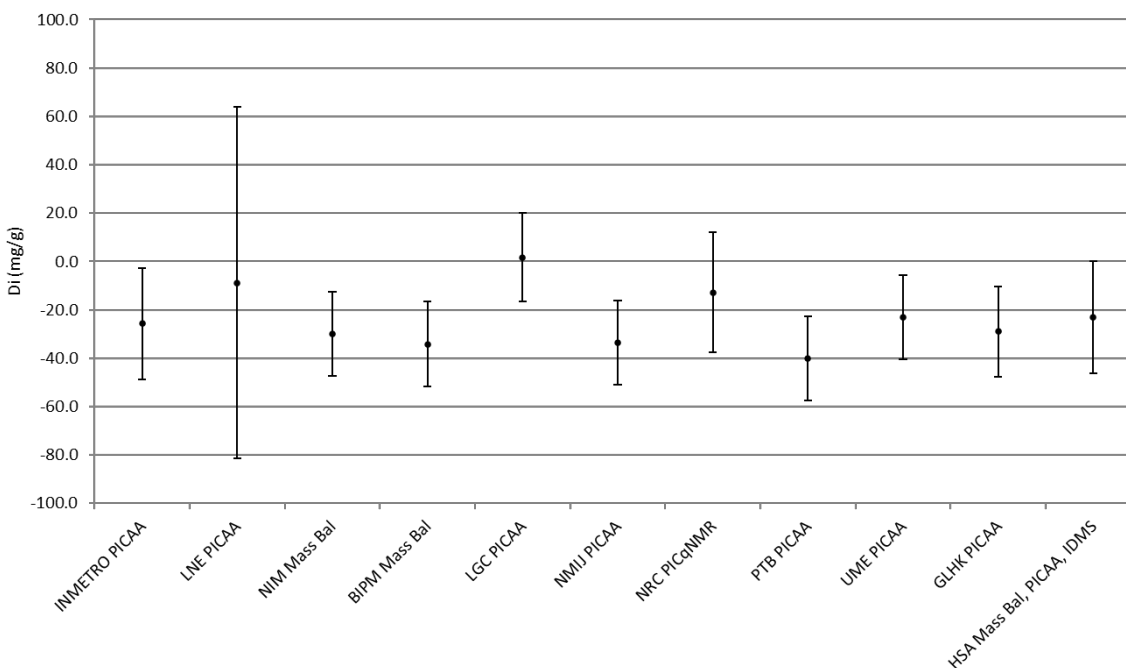


Figure 14: Degree of equivalence with the  $KCRV_{PepImp}$  for total related peptide impurities for each participant. Points are plotted with the associated expanded uncertainty in the degree of equivalence corresponding to a confidence level of about 95 %.

Table 7: Degrees of equivalence  $D_i$  and expanded uncertainties  $U(D_i)$  at a confidence level of about 95 % in mg/g for the  $KCRV_{PepImp}$  for total related peptide impurities

	$D_i$	$U(D_i)$
INMETRO, Brazil	-25.8	22.9
LNE, France	-8.8	72.8
NIM, China	-30.0	17.5
BIPM	-34.1	17.4
LGC, United Kingdom	1.6	18.3
NMIJ, Japan	-33.6	17.3
NRC, Canada	-12.8	24.9
PTB, Germany	-40.2	17.3
UME, Turkey	-23.0	17.5
GLHK, Hong Kong	-29.0	18.6
HSA, Singapore	-23.2	23.2

## Key Comparison Reference Value (KCRV) for the Mass Fraction of VE in CCQM-K115.2018

The  $KCRV_{VE}$  for the mass fraction of VE is based on a mass balance calculation that takes into account the most consistent set of results for the peptide related impurities  $KCRV_{PepImp}$ , TFA mass fraction and the water mass fraction. Contributions from volatile organic solvents, cations and anions other (than TFA) have been found to be negligible [9].

The measurement equation to assign the  $KCRV_{VE}$  of VE in CCQM-K115.2018 (in mg/g) is:

$$w_{VE} = 1000 - (w_{PepImp} + w_{Water} + w_{TFA})$$

$w_{VE}$	= $KCRV_{VE}$ for mass fraction of VE in CCQM-K115.2018
$w_{PepImp}$	= $KCRV_{PepImp}$ for mass fraction of peptide related impurities in CCQM-K115.2018
$w_{Water}$	= Mass fraction of water in CCQM-K115.2018 obtained by the HSA, NRC and BIPM
$w_{TFA}$	= Mass fraction of TFA in CCQM-K115.2018 obtained by the HSA, NIM and BIPM

The standard uncertainty ( $u(KCRV_{VE})$ ) associated with the mass fraction estimate for  $KCRV_{VE}$  is calculated from the equation:

$$u_{w_{VE}} = \sqrt{(u_{w_{PepImp}})^2 + (u_{w_{Water}})^2 + (u_{w_{TFA}})^2}$$

The input values for impurities used for the calculation of  $KCRV_{VE}$  and the corresponding combined standard uncertainty in CCQM-K115.2018 are given in Table 8.

Table 8: Input values for impurities used for the calculation of  $KCRV_{VE}$  and corresponding combined standard uncertainty in CCQM-K115.2018

	$w$ (mg/g)	n	$u_w$ (mg/g)
Peptide related impurities ( $KCRV_{PepImp}$ )	53.0	large	8.6
Water	47.5	large	4.1
TFA	286.7	large	2.3
<b><math>KCRV_{VE}</math></b>	<b>613</b>		<b>10</b>

Figure 15 shows the participant results with their reported standard uncertainties plotted against the  $KCRV_{VE}$  of 613 mg/g for VE in CCQM-K115.2018 (solid line) and its corresponding standard uncertainty of 10 mg/g ( $k = 1$ ). A corresponding expanded uncertainty of 20 mg/g ( $k = 2$ ) at a confidence level of about 95 % was calculated.

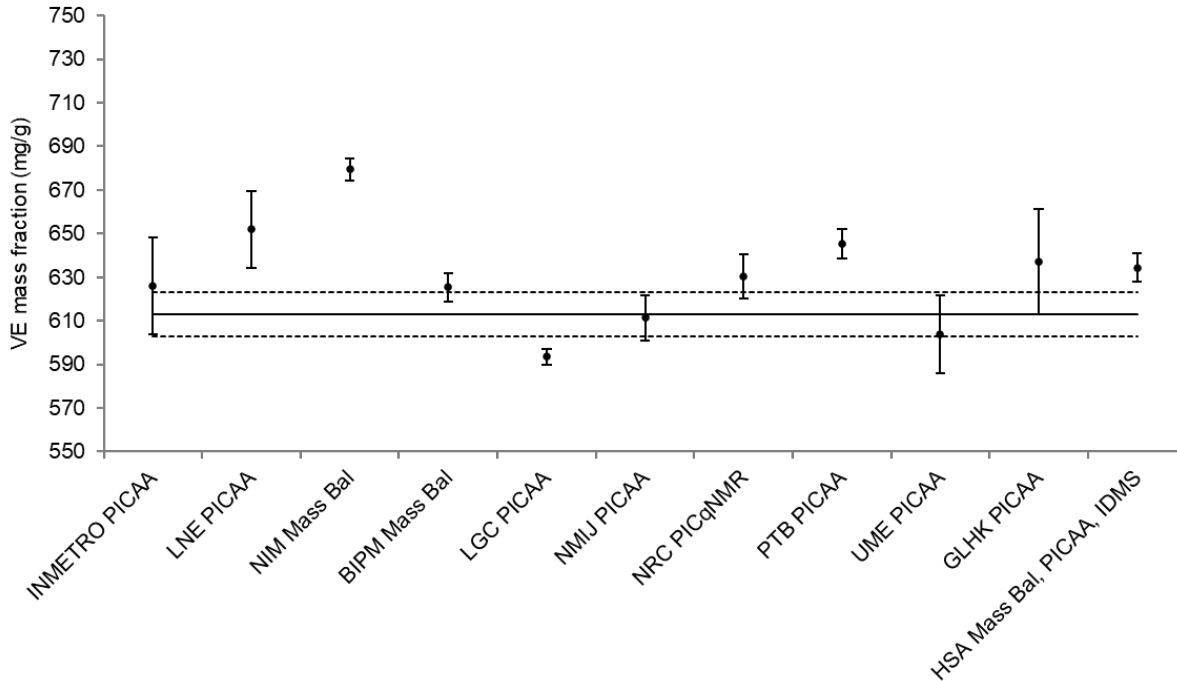


Figure 15: Mass fraction estimates by participants for VE in CCQM-K115.2018 with their reported combined standard uncertainties ( $\pm u_c, k = 1$ ). The  $KCRV_{VE}$  for CCQM-K115.2018 (solid line) is 613 mg/g. The calculated combined standard uncertainty of the  $KCRV_{VE}$  is  $\pm 10$  mg/g. Dashed lines show the  $u(KCRV_{VE})$  ( $k = 1$ ) of the  $KCRV_{VE}$ .

The degree of equivalence of a participant's result with the  $KCRV_{VE}$  ( $D_i$ ) is given by:

$$D_i = w_i - KCRV_{VE}$$

The expanded uncertainty  $U_i$  at a confidence level of about 95 % associated with the  $D_i$  was calculated as [30]:

$$U_{95\%}(D_i) = 2 \cdot \sqrt{u(w_i)^2 + u(KCRV_{VE})^2}$$

Figure 16 indicates the degree of equivalence ( $D_i$ ) of each key comparison participant's result with the  $KCRV_{VE}$  for VE. The corresponding values are listed in Table 9.

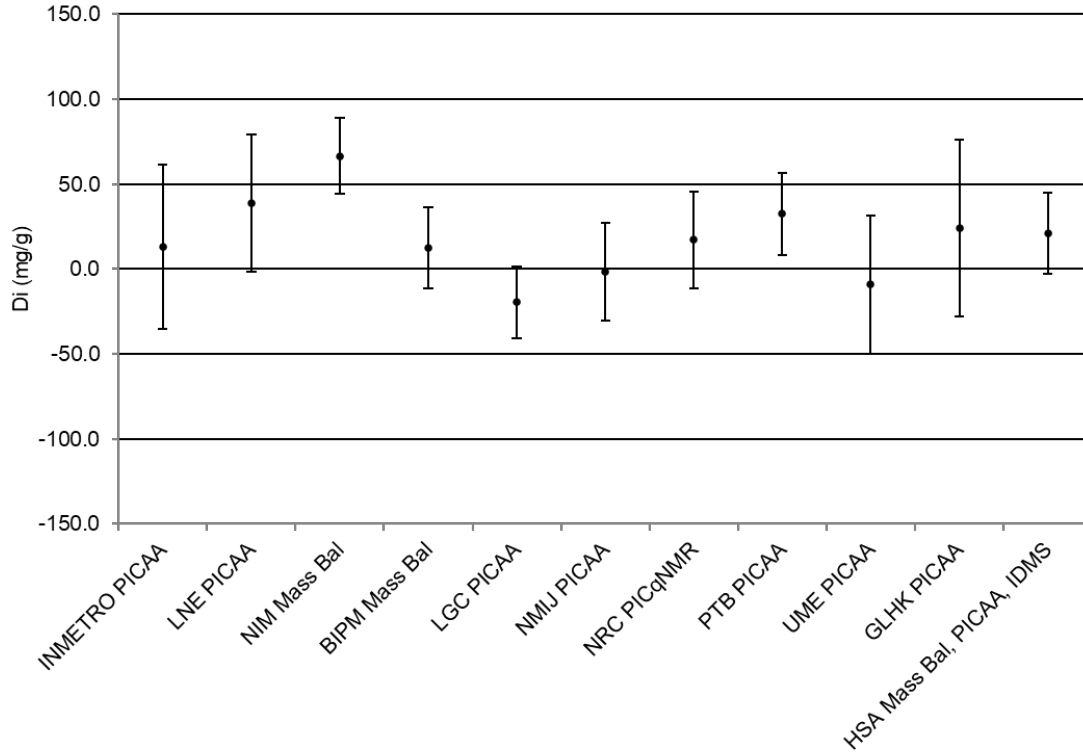


Figure 16: Degree of equivalence with the  $KCRV_{VE}$  for VE for each participant. Points are plotted with the associated expanded uncertainty in the degree of equivalence corresponding to a confidence level of about 95 %.

Table 9: Degrees of equivalence  $D_i$  and expanded uncertainties  $U(D_i)$  at a confidence level of about 95 % in mg/g for the  $KCRV_{VE}$  for VE

	$D_i$	$U(D_i)$
INMETRO, Brazil	13.0	48.3
LNE, France	39.0	40.4
NIM, China	66.5	22.4
BIPM	12.5	23.9
LGC, United Kingdom	-19.5	21.3
NMIJ, Japan	-1.6	28.9
NRC, Canada	17.3	28.4
PTB, Germany	32.4	24.0
UME, Turkey	-9.2	40.8
GLHK, Hong Kong	24.0	52.2
HSA, Singapore	21.3	23.9

## CONCLUSIONS

VE was selected to be representative of chemically synthesized linear peptides of known sequence, without cross-links, up to 5 kDa and without modification. It was anticipated to provide an analytical measurement challenge representative for the value-assignment of compounds of broadly similar structural characteristics.

The majority of participants used a PICAA approach as the amount of material that has been provided to each participant (25 mg) is insufficient to perform a full mass balance-based characterization of the material by a participating laboratory. The coordinators, both the BIPM and the NIM, were the laboratories to use the mass balance approach as they had more material available.

It was decided to propose KCRVs for both the VE mass fraction and the mass fraction of the peptide related impurities as indispensable contributor regardless of the use of PICAA, mass balance or any other approach to determine the VE purity. This allows participants to demonstrate the efficacy of their implementation of the approaches used to determine the VE mass fraction. In particular, it allows participants to demonstrate the efficacy of their implementation of peptide related impurity identification and quantification.

More detailed studies on the identification/quantification of peptide related impurities revealed that the integrity of the impurity profile of the related peptide impurities obtained by the participant is crucial for the impact on accuracy of the VE mass fraction assignment.

Different methods had been investigated to obtain a  $KCRV_{PepImp}$  for the mass fraction of peptide impurities.

The  $KCRV_{PepImp}$  for the mass fraction of peptide impurities is based on the assumption that only the most consistent set of results is taken for the calculation of the  $KCRV_{PepImp}$ . The sum of the combined *cis/trans* VE depsipeptide impurities (only identified/quantified by NRC and confirmed by BIPM and HSA) and mass fractions of peptide related impurities that have been identified by at least two participants have been used to establish the  $KCRV_{PepImp}$ . The corresponding standard uncertainty ( $u(KCRV_{PepImp})$ ) of the  $KCRV_{PepImp}$  is the combined uncertainty of the individual uncertainties provided by the participants for the individual peptide impurities that have been considered. Consequently, the  $KCRV_{PepImp}$  of 53.0 mg/g is associated with a relatively large corresponding expanded uncertainty of  $\pm 17.3$  mg/g ( $k = 2$ ) providing a more realistic basis of evaluation for the capabilities of the participants to identify/quantify peptide related impurities. Inspection of the degree of equivalence plots for the mass fraction of peptide impurities and additional information obtained from the peptide related impurity profile indicates that in all cases the major related peptide impurity, VE depsipeptide, has not been identified. The VE depsipeptide impurity was initially and uniquely identified and quantified by the NRC by the use of  $^1H$ -NMR. The related peptide impurity mass fraction results of only four participants (NRC, LGC, LNE and HSA) are in agreement with the  $KCRV_{PepImp}$ . The NRC has identified and quantified the VE depsipeptide whereas the LGC, LNE and HSA have not identified the VE depsipeptide but accounted for that contribution.

Different methods had also been investigated to obtain a  $KCRV_{VE}$  for the VE mass fraction. The  $KCRV_{VE}$  for the mass fraction of VE is based on a mass balance calculation that takes into account the most consistent set of results for the peptide related impurities  $KCRV_{PepImp}$ , TFA mass fraction and the water mass fraction.

The  $KCRV_{VE}$  for CCQM-K115.2018 is 613 mg/g with a corresponding expanded uncertainty of the  $KCRV_{VE}$  of  $\pm 20$  mg/g ( $k = 2$ ).

The VE material is not sufficiently pure and the corresponding expanded uncertainty is too large to serve as a calibrator to directly support a comparison on the HbA1c quantification in biological samples by IDMS.



## **HOW FAR THE LIGHT SHINES STATEMENT (HFTLS)**

Successful participation in the CCQM-K115.2018 comparison will support CMCs for:

- chemically synthesized peptides of known sequence, without cross-links, up to 5 kDa and without modifications. Additional evidence is required to support claims related to peptides that contain more than 5 kDa, or have been produced using a recombinant process;
- pure peptide primary reference materials value assigned for the mass fraction of the main component peptide within the material;
- methods for the value assignment of the mass fraction of the main component peptide within the material;
- the identification and quantification of minor component peptide impurities within the material.

In addition, the comparison will support traceability statements of CMCs for peptide and protein quantification which are dependent on pure peptide reference materials or methods for their value assignment for peptides meeting the above criteria.

The hexapeptide of HbA0 (VHLTPE or VE) has been proposed as the comparison material, since:

- it will allow the generic capabilities listed above to be demonstrated for non-modified peptides without cross-links and up to 5 kDa molecular mass [1];
- it can be obtained in sufficiently large quantities required for the comparison;
- it will directly support NMI/DI services and certified reference materials currently being provided by NMIs/DIs [31];
- Hemoglobin A1c (HbA1c) is an important analyte for which reference methods have been developed in laboratory medicine [32-37] where VE is the signature peptide for the quantification of HbA0.

## **ACKNOWLEDGEMENTS**

The study coordinators thank all of the participating laboratories for providing all the requested information and excellent collaboration during the course of these studies.

## REFERENCES

- [1] R. D. Josephs, G. Martos, M. Li, L. Wu, J. E. Melanson, M. Quaglia, P. J. Beltrao, D. Prevoo-Franzsen, A. Boeuf, V. Delatour, M. Oztug, J.-S. Jeong, S.-R. Park: Establishment of measurement traceability for peptide and protein quantification through rigorous purity assessment – A review, *Metrologia* **56** (2019) 4, 044006 (29pp).
- [2] J. Marriott, G. O'Connor, H. Parkes: Final Report - Study of Measurement Service and Comparison Needs for an International Measurement Infrastructure for the Biosciences and Biotechnology: Input for the BIPM Work Programme, Rapport BIPM-2011/02 (2011) <http://www.bipm.org/utis/common/pdf/rapportBIPM/2011/02.pdf>
- [3] Strategy 2021-2030: CCQM Working Group on Protein Analysis (PAWG), Consultative Committee for Amount of Substance - Metrology in Chemistry and Biology (CCQM), online access (<https://www.bipm.org/en/committees/cc/ccqm/wg/ccqm-pawg>).
- [4] R. D. Josephs, M. Li, D. Song, S. Westwood, N. Stoppacher, A. Daireaux, T. Choteau, R. I. Wielgosz, P. Xiao, Y. Liu, X. Gao, C. Zhang, T. Zhang, W. Mi, C. Quan, T. Huang, H. Li, R. Flatschart, R. Borges Oliveira, J. E. Melanson, R. Ohlendorf, A. Henrion, T. Kinumi, L. Wong, Q. Liu, M. Oztug Senal, B. Vatansever, I. Ün, A. C. Gören, M. Akgöz, M. Quaglia. J. Warren: Final Report on key comparison CCQM-K115: Peptide Purity - Synthetic Human C-Peptide, *Metrologia* **54** (2017) Tech. Suppl., 1A, 08007.
- [5] R. D. Josephs, M. Li, D. Song, A. Daireaux, T. Choteau, N. Stoppacher, S. Westwood, R. I. Wielgosz, H. Li, J. E. Melanson, M. Akgöz, A. C. Gören, I. Ün, M. Quaglia, J. Warren: Final Report on pilot study CCQM-P55.2: Peptide Purity - Synthetic Human C-Peptide, *Metrologia* **54** (2017) Tech. Suppl., 1A, 08011.
- [6] R. D. Josephs, M. Li, A. Daireaux, T. Choteau, G. Martos, S. Westwood, R. I. Wielgosz, H. Li, S. Wang, X. Li, N. Shi, P. Wu, L. Feng, T. Huang, T. Zhang, S. Li, P. J. Beltrão, A. Marcos Saraiva, B. C. Garrido, S. M. Naressi Scapin, W. Wollinger, Y. Bacila Sade, M.-P. Thibeault, B. B. Stocks, J. E. Melanson, T. Kinumi, M. F. Bin Rezali, M. Öztug, M. Akgöz, M. Quaglia: Key comparison study on peptide purity - synthetic oxytocin, *Metrologia* **57** (2020) Tech. Suppl., 1A, 08014.
- [7] R. D. Josephs, M. Li, A. Daireaux, T. Choteau, G. Martos, S. Westwood, R. I. Wielgosz, H. Li, S. Wang, L. Feng, T. Huang, M. Pan, T. Zhang, N. Gonzalez-Rojano, M. Balderas-Escamilla, A. Perez-Castorena, M. Perez-Urquiza, I. Ün, M. Bilsel: Pilot study on peptide purity - synthetic oxytocin, *Metrologia* **57** (2020) Tech. Suppl., 1A, 08016.
- [8] L. Mackay: CCQM OAWG Strategy Document for Rolling Programme Development, OAWG/13-02 (2013) BIPM webpage, CCQM OAWG working documents.
- [9] S. Westwood, T. Choteau, A. Daireaux, R. D. Josephs, R. I. Wielgosz: Mass Balance Method for the SI Value Assignment of the Purity of Organic Compounds, *Anal. Chem.* **85** (2013) 3118-3126.

- [10] S. Westwood, R. D. Josephs, A. Daireaux, R. I. Wielgosz, S. Davies, H. Wang, J. Rodrigues, W. Wollinger, A. Windust, M. Kang, S. Fuhai, R. Philipp, P. Kuhlich, S.-K. Wong, Y. Shimizu, M. Pérez, M. Avila, M. Fernandes-Whaley, D. Prevoo, B.J. de Vos, R. Visser, M. Archer, T. LeGoff, S. Wood, D. Bearden, M. Bedner, A. Boroujerdi, D. Duewer, D. Hancock, B. Lang, B. Porter, M. Schantz, J. Sieber, E. White, S. A. Wise: Final report on key comparison CCQM-K55.a (estradiol): An international comparison of mass fraction purity assignment of estradiol, *Metrologia* **49** (2012) Tech. Suppl., 1A, 08009.
- [11] S. Westwood, R. D. Josephs, T. Choteau, A. Daireaux, C. Mesquida, R. I. Wielgosz, A. Rosso, M. Ruiz de Arechavaleta, S. Davies, H. Wang, E. C. Pires do Rego, J. Marques Rodrigues, E. de Freitas Guimarães, M. V. Barreto Sousa, T. M. Monteiro, L. Alves das Neves Valente, F. G. Marques Violante, R. R. Ribeiro Almeida, M. C. Baptista Quaresma, R. Nogueira, A. Windust, X. Dai, X. Li, W. Zhang, M. Li, M. Shao, C. Wei, S.-K. Wong, J. Cabillic, F. Gantois, R. Philipp, D. Pfeifer, S. Hein, U.-A. Klyk-Seitz, K. Ishikawa, E. Castro, N. Gonzalez, A. Krylov, T. Tang Lin, L. Tong Kooi, M. Fernandes-Whaley, D. Prévo, M. Archer, R. Visser, N. Nlhapo, B.J. de Vos, S. Ahn, P. Pookrod, K. Wiangnon, N. Sudsiri, K. Muaksang, C. Cherdchu, A. C. Gören, M. Bilsel, T. LeGoff, D. Bearden, M. Bedner, D. Duewer, D. Hancock, B. Lang, K. Lippa, M. Schantz, J. Sieber: Final report on key comparison CCQM-K55.b (aldrin): An international comparison of mass fraction purity assignment of aldrin, *Metrologia* **49** (2012) Tech. Suppl., 1A, 08014.
- [12] S. Westwood, R. D. Josephs, T. Choteau, A. Daireaux, R. Wielgosz, S. Davies, M. Moad, B. Chan, A. Muñoz, P. Conneely, M. Ricci, E. C. Pires do Rego, B. C. Garrido, F. G. M. Violante, A. Windust, X. Dai, T. Huang, W. Zhang, F. Su, C. Quan, H. Wang, M.-F. Lo, W.-F. Wong, F. Gantois, B. Lalere, U. Dorgerloh, M. Koch, U.-A. Klyk-Seitz, D. Pfeifer, R. Philipp, C. Piechotta, S. Recknagel, R. Rothe, T. Yamazaki, O. B. Zakaria, E. Castro, M. Balderas, N. González, C. Salazar, L. Regalado, E. Valle, L. Rodríguez, L. Á. Laguna, P. Ramírez, M. Avila, J. Ibarra, L. Valle, M. Pérez, M. Arce, Y. Mitani, L. Konopelko, A. Krylov, E. Lopushanskaya, T. T. Lin, Q. Liu, L. T. Kooi, M. Fernandes-Whaley, D. Prevoo-Franzsen, N. Nhlapo, R. Visser, B. Kim, H. Lee, P. Kankaew, P. Pookrod, N. Sudsiri, K. Shearman, A. C. Gören, G. Bilsel, H. Yilmaz, M. Bilsel, M. Çergel, F. G. Çoskun, E. Uysal, S. Gündüz, I. Ün, J. Warren, D. W. Bearden, M. Bedner, D. L. Duewer, B. E. Lang, K. A. Lippa, M. M. Schantz, J. R. Sieber: Final report on key comparison CCQM-K55.c (L-(+)-Valine): Characterization of organic substances for chemical purity, *Metrologia* **51** (2014) Tech. Suppl., 1A, 08010.
- [13] S. Westwood, R. D. Josephs, T. Choteau, A. Daireaux, N. Stoppacher, R. I. Wielgosz, S. Davies, E. C. P. do Rego, W. Wollinger, B. C. Garrido, J. L. N. Fernandes, J. M. Lima, R. B. Oliveira, R. C. de Sena, A. Windust, T. Huang, X. Dai, C. Quan, H. He, W. Zhang, C. Wei, N. Li, D. Gao, Z. Liu, M.-F. Lo, W.-F. Wong, D. Pfeifer, M. Koch, U. Dorgerloh, R. Rothe, R. Philipp, N. Hanari, M. F. Rezali, C. M. Salazar Arzate, E. B. Mercado-Pedraza, V. Serrano Caballero, M. Arce Osuna, A. Krylov, S. Kharitonov, E. Lopushanskaya, Q. Liu,

- T. Tang Lin, M. Fernandes-Whaley, L. Quinn, N. Nhlapo, D. Prevoo-Franzsen, M Archer, B.-J. Kim, S.-Y. Baek, S. Lee, J. Lee, S. Marbumrung, P. Kankaew, K. Chaorenpornpukdee, T. Chaipet, K. Shearman, A. C. Gören, S. Gündüz, H. Yılmaz, I. Un, G. Bilsel, C. Clarkson, M. Bedner, J. E. Camara, B. E. Lang, K. A. Lippa, M. A. Nelson, B. Toman, L. L. Yu: Final Report on key comparison CCQM-K55.d: Mass fraction assignment of folic acid in a high purity material, *Metrologia* 55 (2018) Tech. Suppl., 1A, 08013.
- [14] S. Westwood, G. Martos, R. D. Josephs, T. Choteau, R. Wielgosz, S. Davies, M. Moawad, G. Tarrant, B. Chan, M. Alamgir, E. de Rego, W. Wollinger, B. Garrido, J. Fernandes, R. de Sena, R. Oliveira, J. Melanson, J. Bates., P. Mai Le, J. Meija, C. Quan, T. Huang, W. Zhang, R. Ma, S. Zhang, Y. Hao, Y. He, S. Song, H. Wang, F. Su, T. Zhang, H. Li, W.-H. Lam, W.-F. Wong, W.-H. Fung, R. Philipp, U. Dorgerloh, K. Meyer, C. Piechotta, J. Riedel, T. Westphalen, P. Giannikopoulou, C. Alexopoulos, E. Kakoulides, Y. Kitamaki, T. Yamazaki, Y. Shimizu, M. Kuroe, M. Numata, A. Pérez-Castorena, M. Balderas-Escamilla, J. Garcia-Escalante, A. Krylov, A. Mikheeva, M. Beliakov, M. Palagina, I. Tkachenko, S. Spirin, V. Smirnov, T. Tang Lin, C. Pui Sze, W. Juan, L. Wong, T. Lu, Q. Liu, C. Yizhao, S. L. Peng, M. Fernandes-Whaley, D. Prevoo-Franzsen, L. Quinn, N. Nhlapo, D. Mkhize, D. Marajh, S. Chamane, S. Ahn, K. Choi, S. Lee, J. Han, S.-Y. Baek, B. Kim, S. Marbumrung, P. Jongmesuk, K. Shearman, C. Boonyakong, M. Bilsel, S. Gündüz, I. Ün, H. Yılmaz, G. Bilsel, T. Gökçen, C. Clarkson, J. Warren, E Achar: Mass fraction assignment of Bisphenol-A high purity material, *Metrologia* 58 (2021) 1A, 08015.
- [15] C. Pritchard, F. A. Torma, C. Hopley, M. Quaglia, G. O'Connor: Investigating microwave hydrolysis for the traceable quantification of peptide standards using gas chromatography-mass spectrometry, *Anal. Biochem.* 412 (2011) 1, 40-46.
- [16] C. Pritchard, M. Quaglia, C. Mussell, W. I. Burkitt, H. Parkes, G. O'Connor: Fully traceable absolute protein quantification of somatropin that allows independent comparison of somatropin standards, *Clin. Chem.* 55 (2009) 11, 1984-1990.
- [17] W. I. Burkitt, C. Pritchard, C. Arsene, A. Henrion, D. Bunk, G. O'Connor: Toward Systeme International d'Unite-traceable protein quantification: From amino acids to proteins, *Anal. Biochem.* 376 (2008) 2, 242-251.
- [18] C. G. Arsene, R. Ohlendorf, W. Burkitt, C. Pritchard, A. Henrion, G. O'Connor, D. M. Bunk, B. Guettler: Protein Quantification by Isotope Dilution Mass Spectrometry of Proteolytic Fragments: Cleavage Rate and Accuracy, *Anal. Chem.* 80 (2008) 11, 4154-4160.
- [19] C. G. Arsene, A. Henrion, N. Diekmann, J. Manolopoulou, M. Bidlingmaier: Quantification of growth hormone in serum by isotope dilution mass spectrometry, *Anal. Biochem.* 401 (2010) 2, 228-235.
- [20] A. Munoz, R. Kral, H. Schimmel: Quantification of protein calibrants by amino acid analysis using isotope dilution mass spectrometry, *Anal. Biochem.* 408 (2011) 124-131.
- [21] N. Stoppacher, R. D. Josephs, A. Daireaux, S. Westwood, R. I. Wielgosz: Impurity identification and determination for the peptide hormone angiotensin I by liquid

- chromatography – high resolution tandem mass spectrometry and the metrological impact on value assignments by amino acid analysis, *Anal. Bioanal. Chem.* **405** (2013) 8039–8051.
- [22] R. D. Josephs, N. Stoppacher, A. Daireaux, T. Choteau, K. A. Lippa, K. W. Phinney, S. Westwood, R. I. Wielgosz: State-of-the-art and Trends for the SI Traceable Value Assignment of the Purity of Peptides Using the Model Compound Angiotensin I, *Trends Anal. Chem.* **101** (2018) 108-119.
- [23] J. E. Melanson, M. P. Thibeault, B. B. Stocks, D. M. Leek, G. McRae, J. Meija: Purity assignment for peptide certified reference materials by combining qNMR and LC-MS/MS amino acid analysis results: application to angiotensin II, *Anal. Bioanal. Chem.* **410** (2018) 6719–6731.
- [24] T. P. J. Linsinger, J. Pauwels, A. M. H. van der Veen, H. Schimmel, A. Lamberty, Homogeneity and stability of reference materials, *Accred. Qual. Assur.* **6** (2001) 20-25.
- [25] R. DerSimonian, N. Laird: Meta-analysis in clinical trials, *Control. Clin. Trials* **7** (1986) 177–188.
- [26] Calculated using the DerSimonian-Laird estimator of the ‘NIST Consensus Builder’ online app (<https://consensus.nist.gov>).
- [27] L. A. Carpino, E. Krause, C. D. Sferdean, M. Bienert, M. Beyermann: Dramatically enhanced N→O acyl migration during the trifluoroacetic acid-based deprotection step in solid phase peptide synthesis, *Tetrahedron Lett.* **46** (2005) 1361–1364.
- [28] J. Schwochert, C. Pye, C. Ahlback, Y. Abdollahian, K. Farley, B. Khunte, C. Limberakis, A. S. Kalgutkar, H. Eng, M. J. Shapiro, A. M. Mathiowetz, D. A. Price, S. Liras, R. S. Lokey: Revisiting N-to-O acyl shift for synthesis of natural product-like cyclic depsipeptides, *Org. Lett.* **16** (2014) 6088–6091.
- [29] H. Eberhard, O. Seitz: N→O-Acyl shift in Fmoc-based synthesis of phosphopeptides, *Org. Biomol. Chem.* **6** (2008) 1349-1355.
- [30] CCQM/13-22 Guidance note: Estimation of a consensus KCRV and associated Degrees of Equivalence, 12 April 2013 (<http://www.bipm.org>).
- [31] A. Muñoz, I. Zegers, J. Charoud-Got, C. Weykamp, R. Paleari, A. Mosca, U. Kobold, H. Schimmel, H. Emons: Certification of the amount-of-substance fraction of HbA1c versus the sum of HbA0 and HbA1c in haemoglobin: ERM®-AD500/IFCC. ERM-Certification Report, Luxembourg; 2016: EUR 27574 EN [ISBN 978-92-79-53878-0].
- [32] J.-O. Jeppsson, U. Kobold, J. Barr, A. Finke, W. Hoelzel, T. Hoshino, K. Miedema, A. Mosca, P. Mauri, R. Paroni, L. Thienpont, M. Umemoto, C. Weykamp: Approved IFCC reference method for the measurement of HbA1c in human blood, *Clin. Chem. Lab. Med.* **40** (2002) 1, 78–89.
- [33] P. Kaiser, T. Akerboom, L. Dux, H. Reinauer: Modification of the IFCC reference measurement procedure for determination of HbA1c by HPLC-ESI-MS, *Ger. Med. Sci.* **4** (2006) Doc06.

- [34] P. Kaiser, T. Akerboom, P. Molnar, H. Reinauer: Modified HPLC-electrospray ionization/mass spectrometry method for HbA1c based on IFCC reference measurement procedure, *Clin. Chem.* 54 (2008) 6, 1018–1022.
- [35] P. Kaiser, T. Akerboom, R. Ohlendorf, H. Reinauer: Liquid chromatography–isotope dilution–mass spectrometry as a new basis for the reference measurement procedure for hemoglobin A1c determination, *Clin. Chem.* 56 (2010) 5, 750-754.
- [36] F. Braga, M. Panteghini: Standardization and analytical goals for glycosylated hemoglobin measurement, *Clin. Chem. Lab Med.* 51 (2013) 9, 1719–1726.
- [37] Liu H, Wong L, Yong S, Liu Q, Lee TK. Achieving comparability with IFCC reference method for the measurement of hemoglobin A1c by use of an improved isotope-dilution mass spectrometry method, *Anal. Bioanal. Chem.* 407 (2015) 7579–7587.