

**AFRIMETS**

**Supplementary Comparison**

**on**

**Calibration of Dial Gauge**

**(AFRIMETS.L-S6.1.n01)**  
Renamed from (AFRIMETS.L-S5)

**(2019-2022)**

**Final report**

**2024**

**Prepared by:** *Dr.Eng. Ahmed ElMelegy*

*Giza, Egypt*

**Contents**

**Page No.**

ABSTRACT	3
1. INTRODUCTION	4
2. PARTICIPANTS	5
3. FORM OF COMPARISON	6
4. TIMETABLE	6
5. DESCRIPTION OF THE ARTIFACT:	7
6. CALIBRATION METHOD USED BY EACH PARTICIPANT	8
7. CALIBRATION RESULTS	8
8. TRACEABILITY	9
9. ANALYSIS OF THE RESULTS	9
10. CONCLUSION:	16

**Abstract**

National Metrology Institutes from 8 African countries, namely Egypt, Nigeria, Kenya, Tanzania, Zambia, Zimbabwe, Botswana, and Mauritius have participated in an international supplementary comparison on the calibration of Dial Indicators. This comparison was a part of larger supplementary comparison between 13 African countries for the calibration of hand measuring instruments. This larger comparison which was carried out during the period between December 2019 – December 2022 has been piloted by NIS, Egypt and has been registered in BIPM-KCDB database on December 2019 with the identifier AFRIMETS.L-S5. The artifacts have been prepared by NIS, Egypt and measured before sent to circulate between all participant countries in round-robin scheme and returned back again for NIS, Egypt where a final measurement was made for stability check. The main purpose of these comparisons is to support submission of CMCs for calibration of hand length measuring instruments in BIPM-KCDB.

**1. Introduction**

In December 2019, the Egyptian National Institute of Standards (NIS), Egypt has initiated a comparison for the calibration of length hand measuring instruments which is considered the standard activity in most African metrology institutes. It was not possible to conduct comparison for the calibration all length hand measuring instruments, so a number of 6 hand measuring instruments have been selected, which are external micrometer, caliper, dial gauge, setting rods, pin gauges, and feeler gauges. The comparison was carried out during the period from December 2019 to December 2022 and was piloted by NIS, Egypt. The comparison has been registered in BIPM-KCDB database on December 2019 by the identifier AFRIMETS.L-S5 and was given the internal AFRIMET identifier AFRIMETS L11. The comparisons were carried out according to the protocol approved by all participants before initiating the comparison. The artifacts have been prepared and measured by NIS, Egypt before they were circulated between all participant countries in round-robin scheme and returned back again for NIS, Egypt where a final measurement was made for stability check. The main purpose of these comparisons is to support submission of CMCs for calibration of hand length measuring instruments in BIPM-KCDB.

In this report, 11 African countries, namely Egypt, Morocco, Nigeria, Ethiopia, Kenya, Tanzania, Zambia, Zimbabwe, Botswana, Mauritius and South Africa have participated in an international supplementary comparison on the calibration of dial indicators. A dial indicator of 10 mm range was prepared by NIS, Egypt for the comparison.

## 2. Participants

11 African countries, namely Egypt, Morocco, Nigeria, Ethiopia, Kenya, Tanzania, Zambia, Zimbabwe, Botswana, Mauritius and South Africa have participated in an international supplementary comparison on the calibration of dial indicators. NIS, Egypt was acting as the pilot laboratory. The rest of the 13 countries which are Ghana and Malawi did not participate in the Dial Indicator comparison. The list of participants of this comparison are listed in the following table with their details:

**Table 1 shows the participants NMIs in the Dial Indicator comparison**

Nr.	Participant	Correspondence	E-mail Address Phone number	Address
1	NIS (Pilot) (Egypt)	Osama Terra (Organizer)	<a href="mailto:Osama.terra@gmail.com">Osama.terra@gmail.com</a> +201141172900	Tersa Street, Haram, Giza, Egypt. P. code: 12211, P.O. Box: 136 Giza
		Ahmed Elmelegy (Pilot lab.)	<a href="mailto:ahmedme3@yahoo.com">ahmedme3@yahoo.com</a> +201112145450	
2	LPEE/LNM (Morocco)	Lhossain Mechkour	<a href="mailto:mechkour@lpee.ma">mechkour@lpee.ma</a> Tel : +212 5 22 48 87 94	km 7, Route d'El Jadida, Casablanca – Maroc
3	NMI/SON (Nigeria)	Bede Obayi	<a href="mailto:beobayi@yahoo.com">beobayi@yahoo.com</a>	52, Lome Crescent, Zone 7, Wuse, Abuja
4	NMIE (Ethiopia)	Tadesse Gergiso Birhan Tesfaye	<a href="mailto:tdsgrs@gmail.com">tdsgrs@gmail.com</a> <a href="mailto:bire31@yahoo.com">bire31@yahoo.com</a> Tel : +251 116 67 19 69	B67, 1405 Street, Woreda 6, Bole Sub city, Addis Ababa, Ethiopia. P.O. Box: 5722 Addis Ababa
5	KEBS (Kenya)	Calvin Bore	<a href="mailto:borec@kebs.org">borec@kebs.org</a> +254 20 6948 359	Dimensional Laboratory, Kenya Bureau of Standards, P.O. Box 54974 - 00200, Nairobi, Kenya.
6	TBS (Tanzania)	Joseph James Angela Charles	<a href="mailto:mahillajj@yahoo.co.uk">mahillajj@yahoo.co.uk</a> <a href="mailto:joseph.mahilla@tbs.go.tz">joseph.mahilla@tbs.go.tz</a> angela.charles@tbs.go.tz Tel.: + 255 22 2450206	Morogoro/Sam Nujoma Roads, Ubungo, P.O. Box 9524 Dar-es- Salaam
7	ZMA (Zambia)	Daniel Mutale	<a href="mailto:dmmutalezs@gmail.com">dmmutalezs@gmail.com</a>  +260 955135366	Zambia Metrology Agency Plot # 4526 Lechwe House Freedom Way, Lusaka, Zambia. P.O.Box: 30989 Lusaka
8	SIRDC- NMI (Zimbabwe)	Burnhard Gandah	<a href="mailto:bgandah@sirdc.ac.zw">bgandah@sirdc.ac.zw</a> <a href="mailto:burnhardg@gmail.com">burnhardg@gmail.com</a> Tel: +263 778330014	1574 Alpes Road, Technology Drive Hatcliffe P.O. Box 6640 Harare
9	BOBS (Botswana)	Modiriemang Kame Pamidzani Ntima	<a href="mailto:kame@bobstandards.bw">kame@bobstandards.bw</a> <a href="mailto:Ntima@bobstandards.bw">Ntima@bobstandards.bw</a> <a href="mailto:Pamidzani.ntima@gmail.com">Pamidzani.ntima@gmail.com</a> Tel. (+267) 3903200 Tel. (+267) 72607660	Private Bag B0 48 Gaborone

10	MSB (Mauritius)	Tomeswar Pryam Vaneeda Ramasawmy Pallut	<a href="mailto:tpryam@msb.intnet.mu">tpryam@msb.intnet.mu</a> <a href="mailto:vramasawmy@msb.intnet.mu">vramasawmy@msb.intnet.mu</a> +230 433 3648	Mauritius Standards Bureau Villa Road, Moka Postal code – 80805 Mauritius
11	NMISA (South Africa)	Zanele Nzimande Patrick Masina	<a href="mailto:znzimande@nmisa.org">znzimande@nmisa.org</a> <a href="mailto:pmasina@nmisa.org">pmasina@nmisa.org</a> Tel. +27 12 841 2944	Private Bag X34 Lynnwood Ridge Pretoria 0040

### 3. Form of Comparison

The comparison is made according to round robin scheme. All artifacts including the dial indicator are calibrated first at NIS, Egypt then shipped to the next country in the timetable, and so on. Malawi withdrew from the comparison since they were not ready by that time. Since not all countries participated in the 6 calibration activities, participants will differ from one report to the others. For Dial Indicators, only 11 countries participated (shown in blue in figure 1).

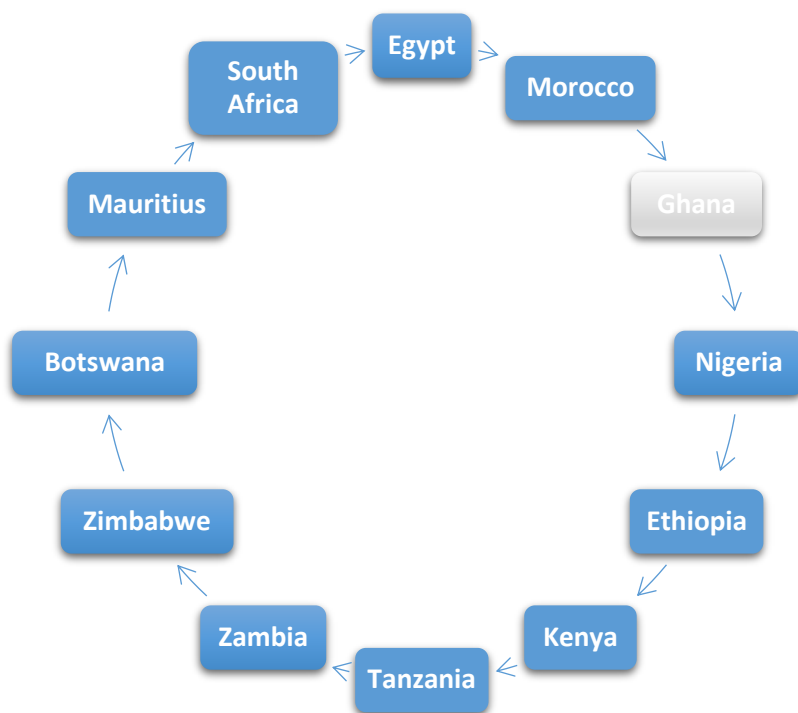


Figure 1: The transportation sequence and measurements of the artifacts.

### 4. Timetable

The sequence of transferring the standards was made according to the protocol. However, delays occur due to the Covid-19 pandemic which took place at the start of the comparison in 2020. Table 2 shows the comparison planned timetable at the protocol. A delay of around one and half year almost from the planned time table.

Table 2 shows the comparison time table at the protocol

Activity	Start Date	End date	Remarks
First calibration at NIS, Egypt	25 November 2019	10 December 2019	
Delivery to LPEE/LNM, Morocco	11 December 2019	31 December 2019	
Calibration at LPEE/LNM, Morocco	1 January 2020	15 January 2020	
Delivery to GSA, Ghana	16 January 2020	5 February 2020	
Calibration at GSA, Ghana	6 February 2020	20 February 2020	
Delivery to NMI/SON, Nigeria	21 February 2020	10 March 2020	
Calibration at NMI/SON, Nigeria	11 March 2020	25 March 2020	
Delivery to NMIE, Ethiopia	26 March 2020	15 April 2020	
Calibration at NMIE, Ethiopia	16 April 2020	30 April 2020	
Delivery to KEBS, Kenya	1 May 2020	20 May 2020	
Calibration at KEBS, Kenya	21 May 2020	5 June 2020	
Delivery to TBS, Tanzania	6 June 2020	26 June 2020	
Calibration at TBS, Tanzania	27 June 2020	12 July 2020	
Delivery to MBS, Malawi	13 July 2020	3 August 2020	Withdrawn
Calibration at MBS, Malawi	4 August 2020	20 August 2020	
Delivery to ZABS, Zambia	21 August 2020	10 September 2020	
Calibration at ZABS, Zambia	11 September 2020	30 September 2020	
Delivery to SIRDC/NMI, Zimbabwe	1 October 2020	20 October 2020	
Calibration at SIRDC/NMI, Zimbabwe	21 October 2020	5 November 2020	
Delivery to BOBS, Botswana	6 November 2020	26 November 2020	
Calibration at BOBS, Botswana	27 November 2020	12 December 2020	
Delivery to MSB, Mauritius	13 December 2020	2 January 2021	
Calibration at MSB, Mauritius	3 January 2021	18 January 2021	
Delivery to NMISA, South Africa	19 January 2021	9 February 2021	
Calibration at NMISA, South Africa	10 February 2021	28 February 2021	
Delivery to NIS, Egypt	1 March 2021	20 March 2021	
Calibration at NIS, Egypt	21 March 2021	5 April 2021	
Final Chance for Submitting the Results	6 April 2021	20 April 2021	
Pre-Draft A	21 April 2021	20 June 2021	

## 5. Description of the artifact:

NIS artifact is a dial indicator as shown in figure 2 that ranges from 0-10 mm.



Figure 2: photograph of Dial Indicators (similar one)

## 6. Calibration method used by each participant

Different methods are used by each participant for the calibration of dial indicators. The used methods by each participant are summarized in table 3.

Table 3 methods used for calibration of Dial Indicators by each participant

Nr.	Participant	Method used for calibration of Dial Indicators
1	NIS (Pilot) (Egypt)	I-checker 2000 Dial calibrator instrument
2	LPEE/LNM (Morocco)	grade K Mitutoyo 122 gauge blocks set
3	NMI/SON (Nigeria)	Grade 0 ceramic gauge block
4	NMIE (Ethiopia)	Not mentioned
5	KEBS (Kenya)	Mitutoyo Automatic DTI tester IC2000
6	TBS (Tanzania)	Gauge block set serial number 061006
7	ZMA (Zambia)	Gauge blocks set
8	SIRDC- NMI (Zimbabwe)	Gauge blocks set s. no. 0905759
9	BOBS (Botswana)	TRIMOS s. no. 1207
10	MSB (Mauritius)	Grade K Gauge blocks set
11	NMISA (South Africa)	Dial Gauge Tester

## 7. Calibration results

The following table (table 4) shows the results for all participant in Dial Indicators calibration comparison. The results of each participant and the calibration uncertainty for the calibration of the Dial Indicators are shown as a single row in table 4.



Table 4. Calibration results by each participant.

	Institute, Country	Nominal	U, mm	Nominal	U, mm	Nominal	U, mm	Nominal	U, mm	Nominal	U, mm
		0.05		0.5		2.1		5.4		10.0	
1	NIS (Egypt) (Pilot)	0.051	0.002	0.501	0.002	2.108	0.002	5.410	0.002	10.013	0.002
2	LPEE/LNM (Morocco)	0.05	0.0084	0.50	0.0084	2.11	0.0084	5.41	0.0084	10.01	0.0084
3	NMI/SON (Nigeria)	N.P.	N.P.	N.P.	N.P.	2.119	0.0103	5.416	0.0093	10.010	0.0058
4	NMIE (Ethiopia)	0.0502	0.0058	0.5001	0.0058	2.0933	0.0058	5.3904	0.0058	9.9903	0.0058
5	KEBS (Kenya)	0.05	0.006	0.50	0.006	N.P.	N.P.	5.4	0.006	10.00	0.006
6	TBS (Tanzania)	N.P.	N.P.	0.51	0.003	2.11	0.003	5.41	0.003	10.01	0.003
7	ZMA (Zambia)	0.05	0.01	0.51	0.01	2.11	0.01	5.41	0.01	10.01	0.01
8	SIRDC- NMI (Zimbabwe)	0.050	0.007	0.505	0.007	2.109	0.007	5.410	0.007	10.012	0.007
9	BOBS (Botswana)	0.05	0.0154	0.50	0.0154	2.11	0.0154	5.40	0.0154	10.01	0.0154
10	MSB (Mauritius)	0.050	0.005	0.510	0.005	2.110	0.005	5.410	0.005	10.010	0.005
11	NMISA (South Africa)	0.05	0.006	0.50	0.006	2.11	0.006	5.41	0.006	10.01	0.006
1	NIS (Egypt) (After)	0.049	0.002	0.502	0.002	2.107	0.002	5.408	0.002	10.013	0.002

N.P.: not participated

## 8. Traceability

Reference for the calibration of the dial Indicators should be traceable to SI unit of length though unbroken traceability chain. The following table demonstrates the traceability of the measurement of each participant that are deduced from the calibration report.

Table 5. Traceability of calibration results by each participant.

Nr.	Participant	Traceability
1	NIS (Egypt)	To SI units of length through NIS primary length standard (He Ne 633 laser)
2	LPEE/LNM (Morocco)	To SI units of length through Mitutoyo Japan Accredited JCSS
3	NMI/SON (Nigeria)	Not mentioned
4	NMIE (Ethiopia)	Not mentioned
5	KEBS (Kenya)	To SI units of length through Mitutoyo standards
6	TBS (Tanzania)	To SI units of length through NMISA standards
7	ZMA (Zambia)	To SI units of length through NMISA standards
8	SIRDC- NMI (Zimbabwe)	To SI units of length through NMISA standards
9	BOBS (Botswana)	To SI units of length through NMISA standards
10	MSB (Mauritius)	To SI units of length through NMISA standards
11	NMISA (South Africa)	To the national measuring standard for length

The status of some NMIs having traceability through NMISA standards did not affect the analysis of comparison results.

## 9. Analysis of the results

### 9.1. Transportation Stability

Drifts of the artifact's values can occur during the transportation of the artifacts and handling over the long period of comparison. Therefore, a stability check must be performed to assure that this change will not affect the comparison results. The instability of the artifacts is assessed according to the following equation:

$$\Delta_{ins} = |x_{NIS_2} - x_{NIS_1}|$$

where,  $x_{NIS_2}$  is the measurement of the pilot (NIS, Egypt) after the comparison and  $x_{NIS_1}$  is the measurement of the pilot before the comparison. The instability of each artifact during the transportation will add additional contribution to the uncertainty of the reference value:

$$u_{ad}(x_i) = \frac{\Delta_{ins}}{2\sqrt{3}}$$

Additional criteria are applied to ensure the stability of the results which is:

$$\Delta_{ins} \leq 0.9 \sqrt{u_{CRV}^2 + u_{min}^2}$$

where, the  $u_{CRV}$  is the uncertainty in the comparison reference value and  $u_{min}$  is the uncertainty of the participant with the lowest uncertainty.

Therefore, the total combined uncertainty for each participant after adding the uncertainty due to the stability will be

$$u_a^2(x_i) = u^2(x_i) + u_{ad}^2(x_i)$$

**Table 6. Stability measurement for each artifact**

Nominal length, (mm)	$\Delta_{ins}$ (mm)	$u_{ad}(x_i)$ mm	$0.9 \sqrt{u_{CRV}^2 + u_{min}^2}$ mm	Status
<b>0.05</b>	<b>0.0020</b>	<b>0.0006</b>	<b>0.00228</b>	<b>Fulfilled</b>
<b>0.5</b>	<b>0.0010</b>	<b>0.0003</b>	<b>0.00231</b>	<b>Fulfilled</b>
<b>2.1</b>	<b>0.0060</b>	<b>0.0017</b>	<b>0.00231</b>	<b>Fulfilled</b>
<b>5.4</b>	<b>0.0020</b>	<b>0.0006</b>	<b>0.00220</b>	<b>Fulfilled</b>
<b>10.0</b>	<b>0.0000</b>	<b>0.0000</b>	<b>0.00220</b>	<b>Fulfilled</b>

**Table 7. correction of combined uncertainties for each participant**

Nr.	Institute, Country	Nominal 0.05	$u_a(x_i)$ , mm	Nominal 0.5	$u_a(x_i)$ , mm	Nominal 2.1	$u_a(x_i)$ , mm	Nominal 5.4	$u_a(x_i)$ , mm	Nominal 10.0	$u_a(x_i)$ , mm
1	NIS (Egypt) (Pilot)	0.0510	0.0012	0.5010	0.0010	2.1080	0.0020	5.4100	0.0012	10.0130	0.0010
2	LPEE/LNM (Morocco)	0.0500	0.0042	0.5000	0.0042	2.1100	0.0045	5.4100	0.0042	10.0100	0.0042
3	NMI/SON (Nigeria)	N.P.	N.P.	N.P.	N.P.	2.1190	0.0054	5.4160	0.0047	10.0100	0.0029
4	NMIE (Ethiopia)	0.0502	0.0030	0.5001	0.0029	2.0933	0.0034	5.3904	0.0030	9.9903	0.0029
5	KEBS (Kenya)	0.0500	0.0031	0.5000	0.0030	N.P.	N.P.	5.4000	0.0031	10.0000	0.0030
6	TBS (Tanzania)	N.P.	N.P.	0.5100	0.0015	2.1100	0.0023	5.4100	0.0016	10.0100	0.0015
7	ZMA (Zambia)	0.0500	0.0050	0.5100	0.0050	2.1100	0.0053	5.4100	0.0050	10.0100	0.0050
8	SIRDC- NMI (Zimbabwe)	0.0500	0.0035	0.5050	0.0035	2.1090	0.0039	5.4100	0.0035	10.0120	0.0035
9	BOBS (Botswana)	0.0500	0.0077	0.5000	0.0077	2.1100	0.0079	5.4000	0.0077	10.0100	0.0077
10	MSB (Mauritius)	0.0500	0.0026	0.5100	0.0025	2.1100	0.0030	5.4100	0.0026	10.0100	0.0025
11	NMISA (South Africa)	0.0500	0.0031	0.5000	0.0030	2.1100	0.0035	5.4100	0.0031	10.0100	0.0030

**9.2. Reference value of the comparison**

The CRV (comparison reference value) was calculated using the weighted mean method according to the equation:

$$x_{CRV} = \sum_{i=1}^N w_i x_i$$

Where  $w_i$  is the weights and is calculated by the equation:

$$w_i = \frac{u_a^{-2}(x_i)}{\sum_{i=1}^N u_a^{-2}(x_i)}$$

and where  $u_a^2$  is the uncertainty contribution of each participant including the uncertainty due to the stability analysis: The standard uncertainty in the CRV value is calculated according to the following equation:


$$u(x_{CRV}) = \frac{\sqrt{\sum_{i=1}^N \frac{u^2(x_i)}{u_a^4(x_i)}}}{\sum_{i=1}^N u_a^{-2}(x_i)}$$

Calculation of the CRV and its uncertainty are given in table 6 and figure 2. The calculation is made after removing the inconsistent data according to section 9.3.


**Table 8. Comparison CRV and its uncertainty**

<b>Nominal length, (mm)</b>	<b>CRV value (length) (mm)</b>	<b>Expanded Uncertainty (@ K=2), (mm)</b>
<b>0.05</b>	0.05054	0.00155
<b>0.50</b>	0.50119	0.00161
<b>2.10</b>	2.10969	0.00162
<b>5.40</b>	5.40944	0.00140
<b>10.00</b>	10.01230	0.00141


## Final report: Calibration of Dial Gauge

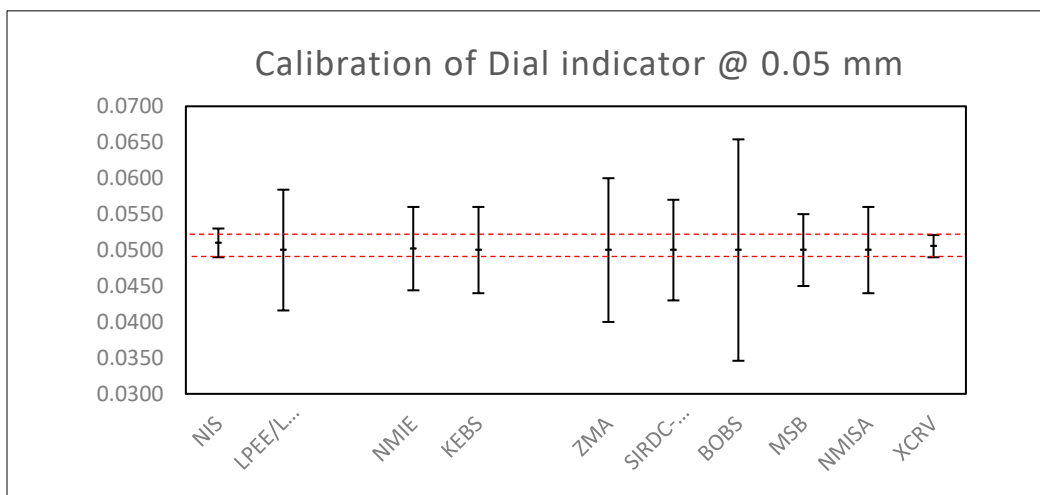


a)

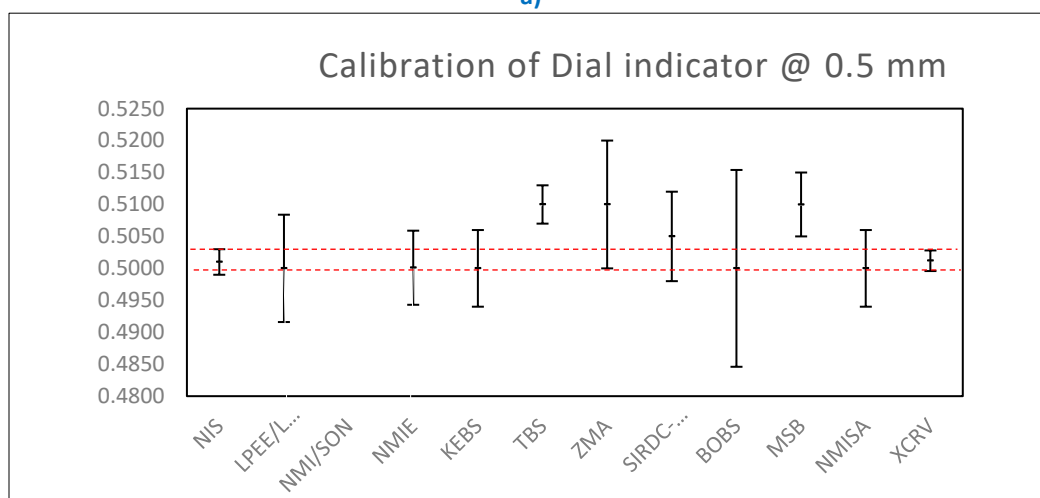


b)

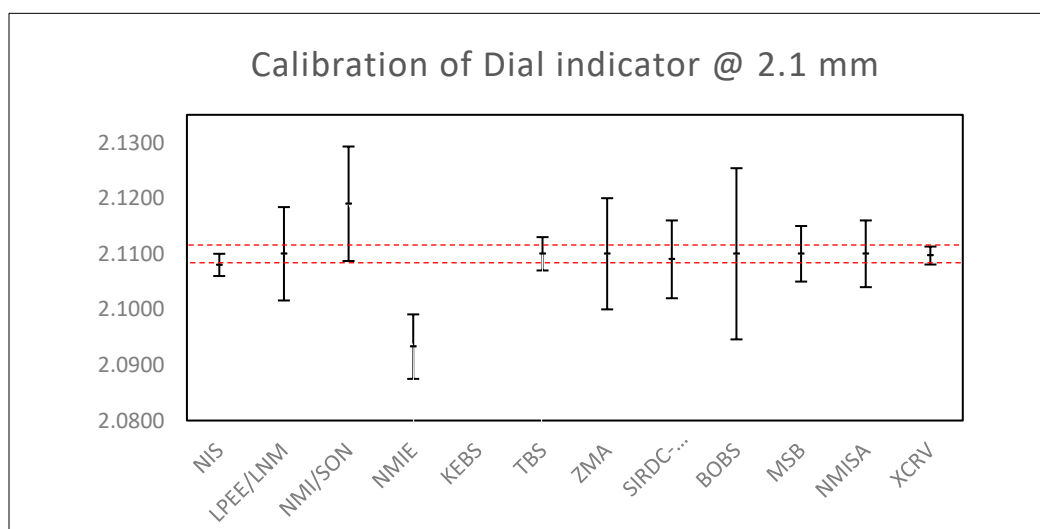

c)

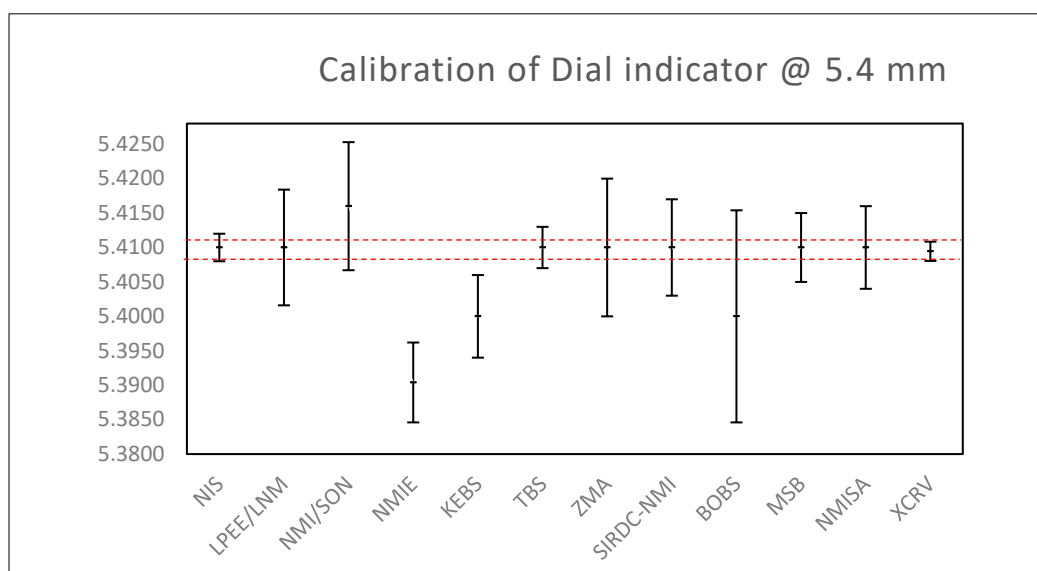

d)

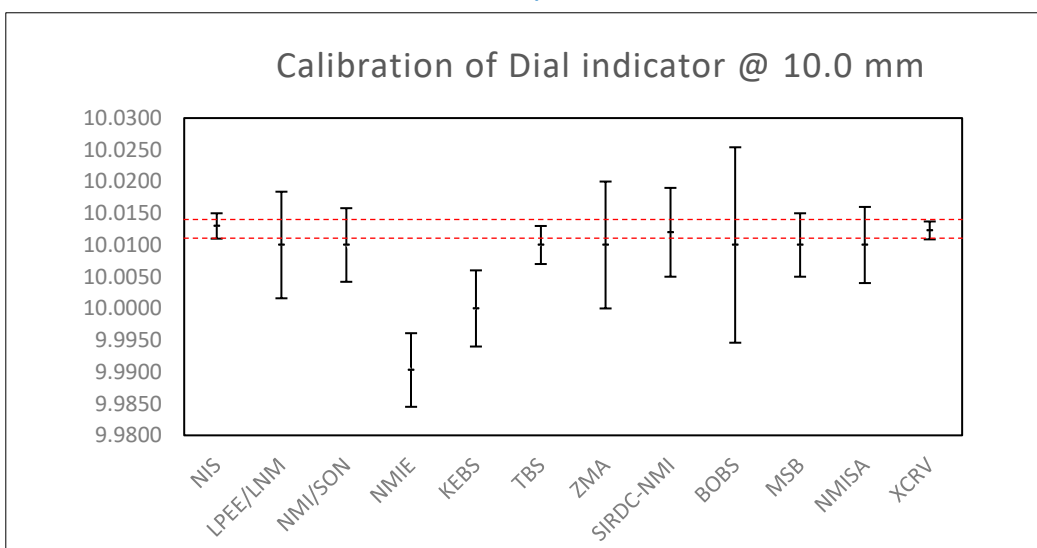

e)

Figure 3. The results of the participants in comparison with the CRV and it's uncertainty (expanded), a, b, c, d & e.

### 9.3. Consistency check of the results

Before calculating the CRV and its uncertainty a consistency of the comparison results must be examined. To determine the consistency of comparisons results Chi-square value  $\chi^2_{obs}$  is calculated according to the following equation:

$$\chi_{obs}^2 = \sum_{i=1}^n \frac{(x_i - x_{CRV})^2}{u_a^2(x_i)} \quad 3$$

For the data to be consistent, the following condition must satisfy

$$\Pr\{\chi^2(v) > \chi_{obs}^2\} < 0.05 \quad 4$$

Where  $v$  is the degrees of freedom which is the number of participant and  $P_r$  denotes “probability of” and  $\chi^2(v)$  is the inverse of the chi-square cumulative distribution function with degree of freedom specified by  $v$  for the probability of 0.05 (corresponding to the 95 % level of confidence). In this case, the participant with the highest value of  $\chi_{obs}^2$  is excluded from the next round of evaluation and a new reference value, reference standard uncertainty, and chi-squared values are calculated again without the excluded laboratory. If the consistency check did not fail then  $y$  was accepted as the  $x_{CRV}$  and the  $u(x_{CRV})$  are accepted. The number of participants  $N$ , therefore, the degrees of freedom  $v = N - 1$ . From the Chi-Square table at 95% confidence level, we obtain  $\chi_{0.05}^2$  as tabulated depending on number of participants in each thickness measurement.

**Table 9: Consistency check (Not satisfied)**

Nominal thickness, (mm)	$\chi_{obs}^2$	$\chi_{0.05}^2$	$v$	Consistency $\chi_{obs}^2 \leq \chi_{0.05}^2$ ?
<b>0.05</b>	<b>0.334</b>	<b>15.51</b>	<b>8</b>	<b>Satisfied</b>
<b>0.5</b>	<b>37.282</b>	<b>16.92</b>	<b>9</b>	<b>Not Satisfied</b>
<b>2.1</b>	<b>25.017</b>	<b>16.92</b>	<b>9</b>	<b>Not Satisfied</b>
<b>5.4</b>	<b>52.421</b>	<b>18.31</b>	<b>10</b>	<b>Not Satisfied</b>
<b>10.0</b>	<b>61.733</b>	<b>18.31</b>	<b>10</b>	<b>Not Satisfied</b>

- The results from the following participants are removed before calculating the CRV and its uncertainty for the data to be consistent
  - Participants of TBS & MSB @ (0.5 mm)
  - Participant of NMIE @ (2.1 mm)
  - Participant of NMIE @ (5.4 mm)
  - Participants of NMIE & KEBS @ (10.0 mm)

After removing these results from the CRV calculation; the consistency check:

Table 10: Consistency check (satisfied)

Nominal thickness, (mm)	$\chi_{obs}^2$	$\chi_{0.05}^2$	$\nu$	Consistency $\chi_{obs}^2 \leq \chi_{0.05}^2$ ?
0.5	4.861	14.07	7	Satisfied
2.1	3.728	15.51	8	Satisfied
5.4	13.495	16.92	9	Satisfied
10.0	10.090	15.51	8	Satisfied

#### 9.4. Performance Evaluation

The purpose of the evaluation of performance methods is to provide a normalized performance evaluation so that all results are comparable and the performance of each participant can be measured. In such calibration schemes, the performance of the participants is evaluated by measuring whether the results of the participants are within the uncertainty of the CRV. The performance is evaluated using the normalized error number  $E_n$ , where;

$$E_n = \frac{(x_i - x_{CRV})}{\sqrt{U_{a_i}^2 + U_{CRV}^2}}$$

Where;  $x_i$  and  $U_{a_i}$  are the result and its corresponding adjusted expanded uncertainty of each participant, respectively.  $x_{CRV}$  and  $U_{CRV}$  are the CRV and its expanded uncertainty, respectively.  $E_n$  is interpreted as follows:

$|E_n| \leq 1 \rightarrow$  Satisfactory performance

$|E_n| > 1 \rightarrow$  Unsatisfactory performance

Table 11. Evaluation of performance for the participants using  $E_n$

Nominal length, (mm)	$ E_n $										
	NIS	LPEE/LNM	NMI/SON	NMIE	KEBS	TBS	ZMA	SIRDC-NMI	BOBS	MSB	NMISA
0.05	0.2	0.1	N.E.	0.1	0.1	N.E.	0.1	0.1	0.0	0.1	0.1
0.5	0.1	0.1	N.E.	0.2	0.2	2.6	0.9	0.5	0.1	1.7	0.2
2.1	0.7	0.0	0.9	2.7	N.E.	0.1	0.0	0.1	0.0	0.1	0.1
5.4	0.2	0.1	0.7	3.2	1.5	0.2	0.1	0.1	0.6	0.1	0.1
10.0	0.3	0.3	0.4	3.7	2.0	0.7	0.2	0.0	0.1	0.4	0.4

N.E.: not evaluated

## **10. Conclusion:**

- The results from 8 National Metrology Institutes from Egypt, Morocco Nigeria, Ethiopia, Kenya, Tanzania, Zambia, Zimbabwe, Botswana, Mauritius and South Africa have participated in an AFRIMET supplementary comparison on the calibration of Dial Indicators. The comparison reference value has obtained from the results using the weighted mean method after performing consistency check of the results using the Chi-square method. The Normalized error number  $E_n$  is used to evaluate the performance of all participants. All results are found satisfactory except:
  - NMIE at 2.1 mm, 5.4 mm and 10 mm.
  - KEBS at 5.4 mm and 10 mm.
  - TBS at 0.5 mm.
  - MSB at 0.5 mmare found unsatisfactory ( $E_n > 1$ ).
- The country of Nigeria does not report its measurements for points 0.05 and 0.5 mm, so it is not evaluated at these points.
- The countries of Tanzania does not report its measurements for points 0.05 mm, so it is not evaluated at this point.
- The countries of Kenya does not report its measurements for points 2.1 mm, so it is not evaluated at this point.

## **List of References**

- [1] Guide to preparation of Key Comparison Reports in Dimensional Metrology (GD3), A Lewis, T Coveney 30 Nov 2020.
- [2] Measurement comparisons in the CIPM MRA, Guidelines for organizing, participating and reporting, CIPM MRA-G-11
- [3] M. G. Cox, "The evaluation of key comparison data", metrologia, 39, 589-595, 2002.