

Consultative Committee for Thermometry: CCT K9, SPRT calibration from the Ar TP to the Zn FP

NIST contributors:

T. Herman

M. Chojnacky

W. Guthrie


G. Strouse

Key Comparison 9: SPRT calibration from the Ar TP to the Zn FP

Key Comparison 9 Protocol

ITS-90 SPRT Calibration from the Ar TP to the Zn FP

Method: Collapsed Star

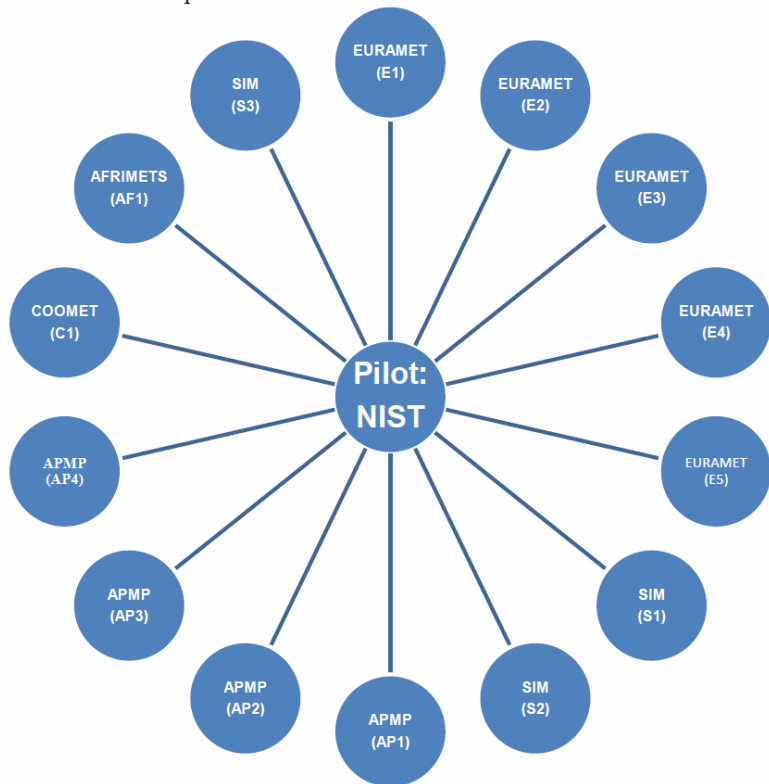

Objective: This comparison is designed to compare the realization of the ITS-90 through the calibration of SPRTs. The range of temperature covered in this comparison is from the triple point of Ar (83.8058 K) to the freezing point of Zn (692.677 K). The transfer standards used will be long-stem SPRTs.

Projected Timeline:

Protocol Agreement
Transfer Standards Sent to NIST
Transfer Standards Returned to NMIs
Transfer Standards Re-Measured by NMIs
Draft A Report Completed

January 31, 2011

~~March 31, 2011~~ **2011-2015**

~~September 30, 2011~~ **2012-2015**

~~December 31, 2011~~ **2012-2015**

~~March 31, 2012~~ **2020**

Toby joined NIST
thermometry team

CCT-K9 meeting held on 17-09-2020, Draft A achieved

- ◆ 2 ITS-90 calibrated SPRTs
 - NMI participant will select their own SPRTs based on their own criteria for suitability and will convey the selection criteria to the Pilot Laboratory
 - SPRTs must be calibrated by NMI participant before measurements are made by the pilot and then again on return from the pilot
 - SPRTs are to be measured at every available fixed-point over the range of the comparison including the In FP and Ga MP
 - The calibration of SPRTs by an NMI participant is to be performed by either fixed-point cells or by comparison with an ITS-90 calibrated reference SPRT

Participating NMIs

NMI Participants:



Pilot:	NIST, Gregory Strouse, gstrouse@nist.gov
AFRIMETS:	NMISA, Hans Liedberg, hliedber@nmisa.org
APMP:	KRISS, Inseok Yang, iyang@kriss.re.kr
APMP:	NIM, Jianping Sun (孙建平), sunjp@nim.ac.cn
APMP:	NMIJ, Jun Tamba, j-tamba@aist.go.jp
APMP:	NMIA, Kim Nguyen, kim.nguyen@measurement.gov.au
COOMET:	VNIIM, Anatoly Pokhodun, a.i.pokhodun@vniim.ru
EURAMET:	NPL, Helen McEvoy, helen.mcevoy@npl.co.uk
EURAMET:	VSL, Andrea Peruzzi, aperuzzi@vsl.nl
EURAMET:	PTB, Joachim Fischer, joachim.fischer@ptb.de
EURAMET:	INRIM, Peter Steur, p.steur@inrim.it
EURAMET:	LNE-INM/CNAM, Yves Hermier, hermier@cnam.fr
SIM:	INMETRO, Renato Nunes Teixeira, rnteixeira@inmetro.gov.br
SIM:	INTI, Javier Skabar, jskabar@inti.gob.ar
SIM:	NRC, Ken Hill, ken.hill@nrc-cnrc.gc.ca

Attendance at Sept. 17, 2020 Meeting


Tobias Herman (NIST),
Giuseppina Lopardo (INRiM),
Javier Garcia Skabar (INTI),
Fernando Sparasci (LNE/CNAM),
Inseok Yang (KRISS),
Jintao Zhang (NIM),
Jianping Sun (NIM),
Eric vd Ham (NMIA),
Mong-Kim Ho (NMIA),
Tohru Nakano (NMIJ),
Jonathan Pearce (NPL),
Sergey Dedyulin (NRC),
Steffen Rudtsch (PTB),
Victor Fuksov (VNIIM),
Conny Barendregt (VSL),
Gijs Snijders (VSL),
Andrea Peruzzi (CCT WG-KC chair).

Measurement Scheme at NIST

Stabilize

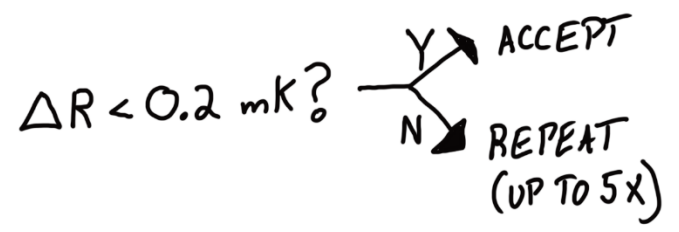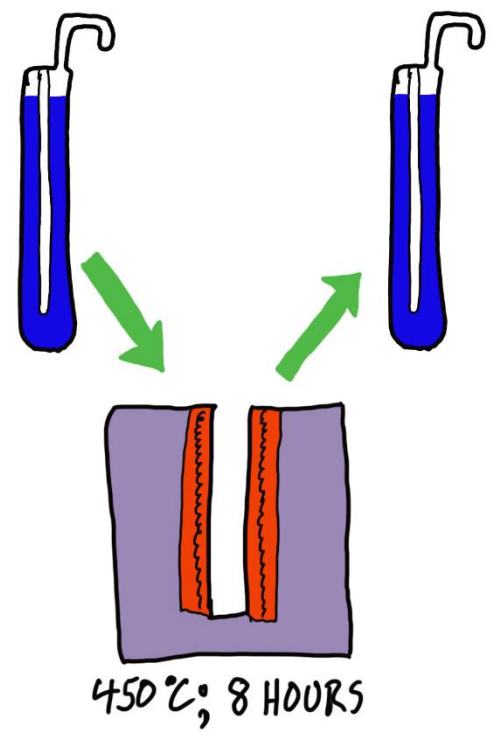

Measure

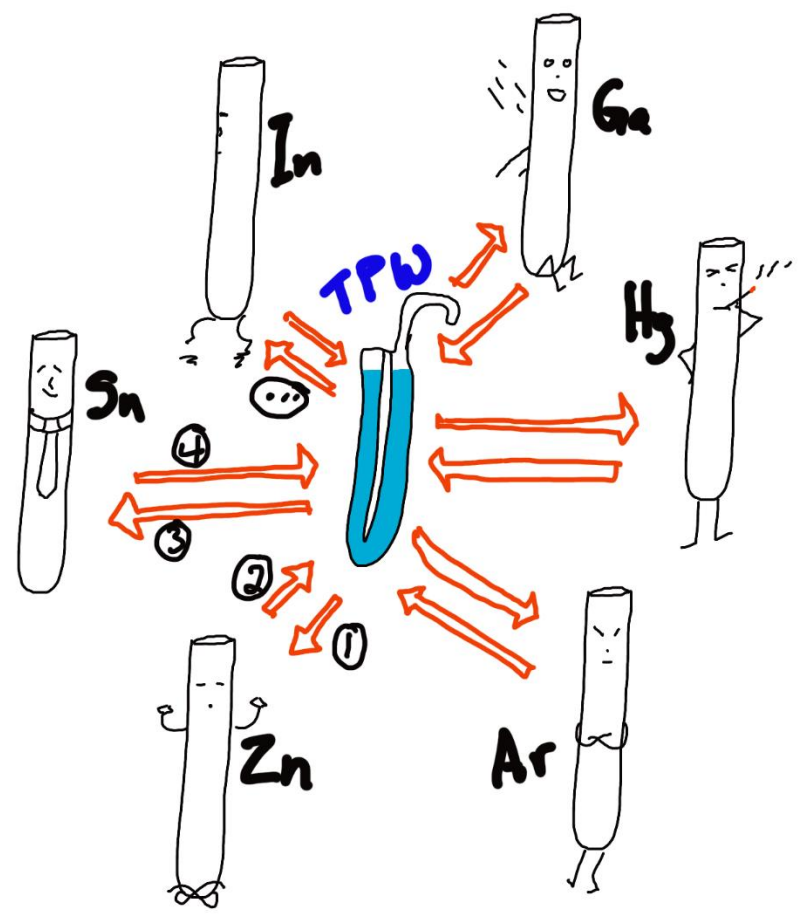

Cutoff criteria and SPRTs rejected

Which SPRTs will contribute to the KCRV?

Criterion 1

$$\left| \frac{W_i^{Post} - W_i^{Ante}}{(dW_r/dT) \sqrt{u_R^2(W_i^{Post}) + u_R^2(W_i^{Ante})}} \right| > t_{0.975, \nu_{eff}}$$



Criterion 2

$$u(C_i) = \frac{1}{2\sqrt{3}} \frac{|W_i^{Post}(FP) - W_i^{Ante}(FP)|}{(dW_r(ITS - 90)/dT)}$$

$$u^2(C_i) \geq \frac{u^2(\Delta T_{NMI_i})}{10}$$



NMI		Zn		Sn		In		Ga		Hg		Ar	
		I	II	I	II	I	II	I	II	I	II	I	II
acer	SPRT1	×	×	×	×	×	×	×	×	✓	✓	×	×
	SPRT2	✓	✓	✓	✓	×	✓	✓	✓	×	×	×	×
asarum	SPRT1	×	✓	×	×	×	✓	×	✓	×	✓	×	✓
	SPRT2	×	✓	×	✓	×	✓	✓	✓	×	✓	×	✓
asimina	SPRT1	-	-	-	-	-	-	-	-	✓	×	✓	✓
	SPRT2	×	✓	✓	✓	×	×	✓	×	×	×	✓	✓
cercis	SPRT1	✓	×	✓	×	✓	✓	✓	✓	✓	✓	✓	✓
	SPRT2	✓	×	✓	×	✓	✓	✓	✓	✓	✓	✓	✓
cornus	SPRT1	✓	✓	✓	✓	✓	✓	✓	✓	✓	✓	✓	✓
	SPRT2	-	-	-	-	-	-	-	-	-	-	-	-
corylus	SPRT1	-	-	-	-	-	-	-	-	-	-	-	-
	SPRT2	-	-	-	-	-	-	-	-	-	-	-	-
	SPRT3	-	-	-	-	-	-	-	-	-	-	-	-
crocus	SPRT1	-	-	-	-	-	-	✓	✓	-	-	-	-
	SPRT2	-	-	-	-	-	-	✓	✓	-	-	-	-
ilex	SPRT1	-	-	✓	✓	✓	✓	✓	✓	✓	✓	×	✓
	SPRT2	×	✓	×	✓	✓	✓	✓	✓	✓	✓	×	×
iris	SPRT1	✓	✓	✓	✓	✓	✓	✓	✓	✓	✓	✓	✓
	SPRT2	✓	✓	✓	✓	×	✓	✓	✓	✓	✓	✓	✓
picea	SPRT1	✓	✓	×	×	×	×	×	×	×	×	✓	✓
	SPRT2	✓	✓	×	×	×	×	×	×	×	×	×	×
prunus	SPRT1	✓	✓	×	×	✓	✓	✓	✓	✓	✓	✓	✓
	SPRT2	✓	✓	✓	-	✓	✓	×	×	✓	✓	✓	✓
quercus	SPRT1	×	×	×	×	×	×	×	×	✓	✓	✓	✓
	SPRT2	×	✓	×	✓	×	✓	×	✓	✓	✓	×	×
rosa	SPRT1	×	✓	×	✓	×	✓	×	×	-	-	-	-
	SPRT2	×	✓	✓	✓	×	✓	×	×	-	-	-	-
silene	SPRT1	×	×	×	×	✓	×	✓	✓	×	✓	×	✓
	SPRT2	×	✓	✓	✓	✓	✓	✓	×	✓	✓	✓	✓
tulipa	SPRT1	×	✓	✓	✓	×	×	×	×	×	✓	×	✓
	SPRT2	×	✓	×	✓	×	✓	×	×	✓	✓	✓	✓
# passes:		10	18	12	14	10	18	15	15	15	18	13	18
# fails:		13	5	12	9	14	6	11	11	8	5	10	5

Zn and Sn

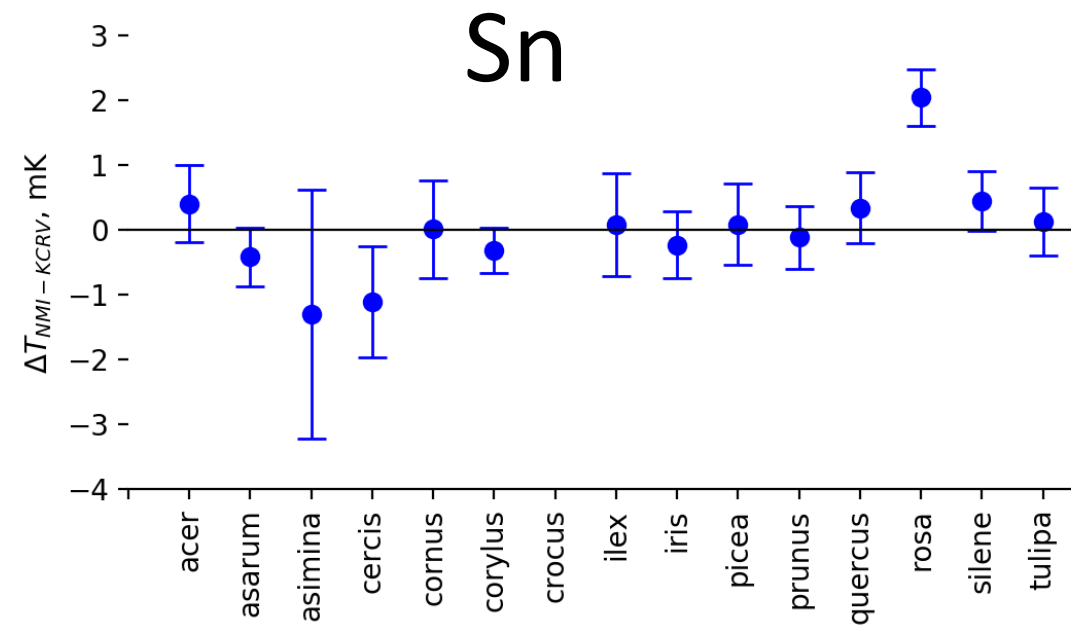
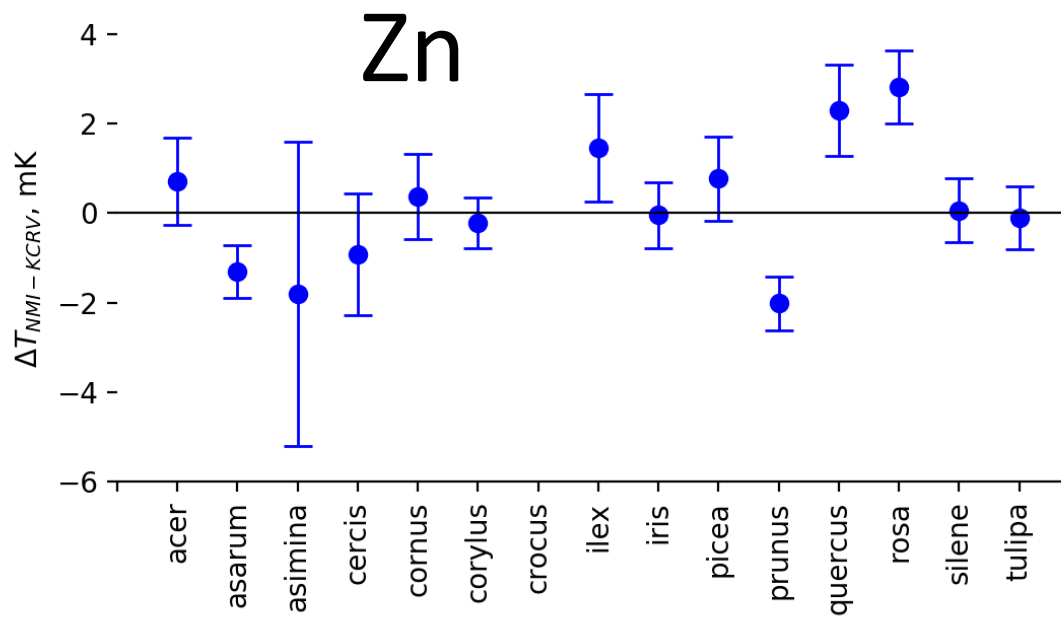


$k=2$ uncertainties of each NMI

In and Ga

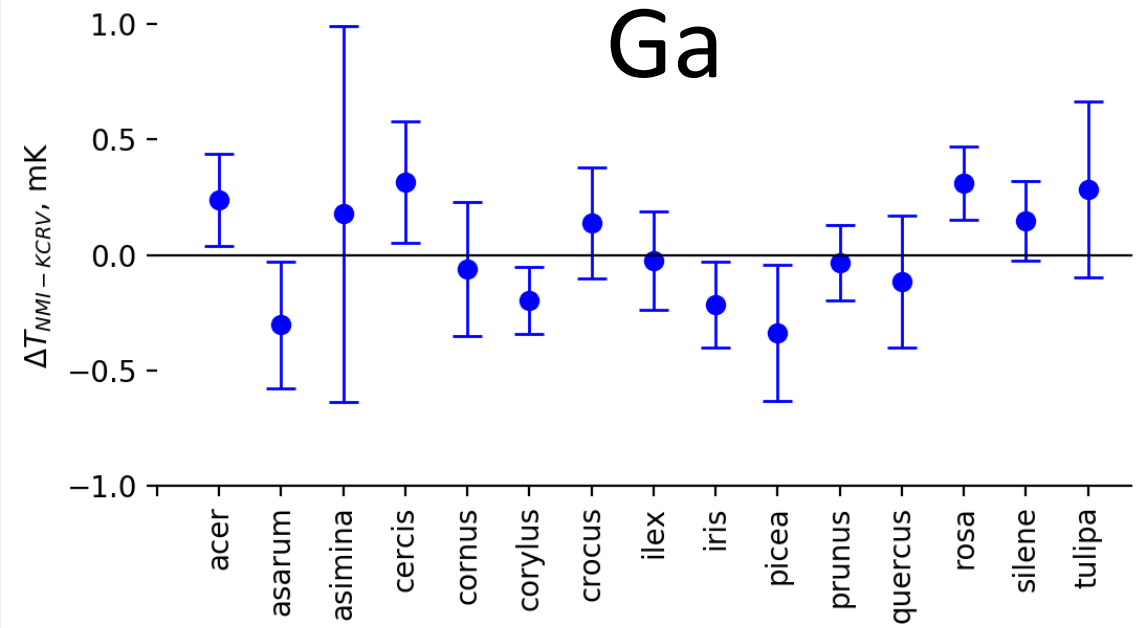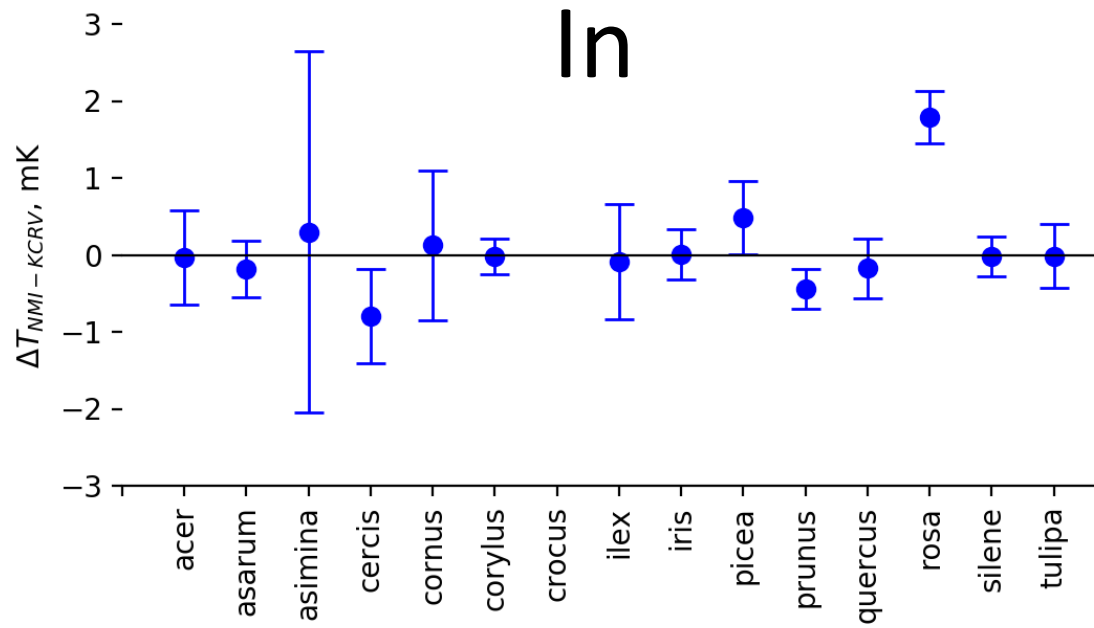

Hg and Ar

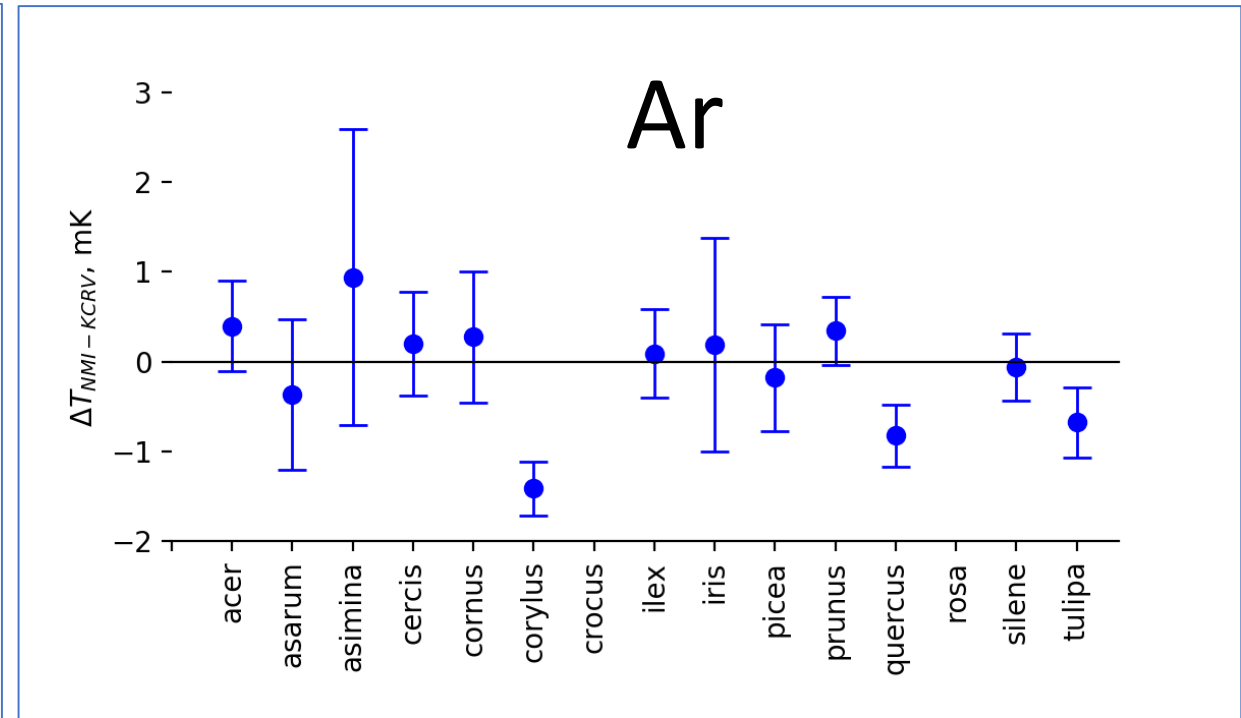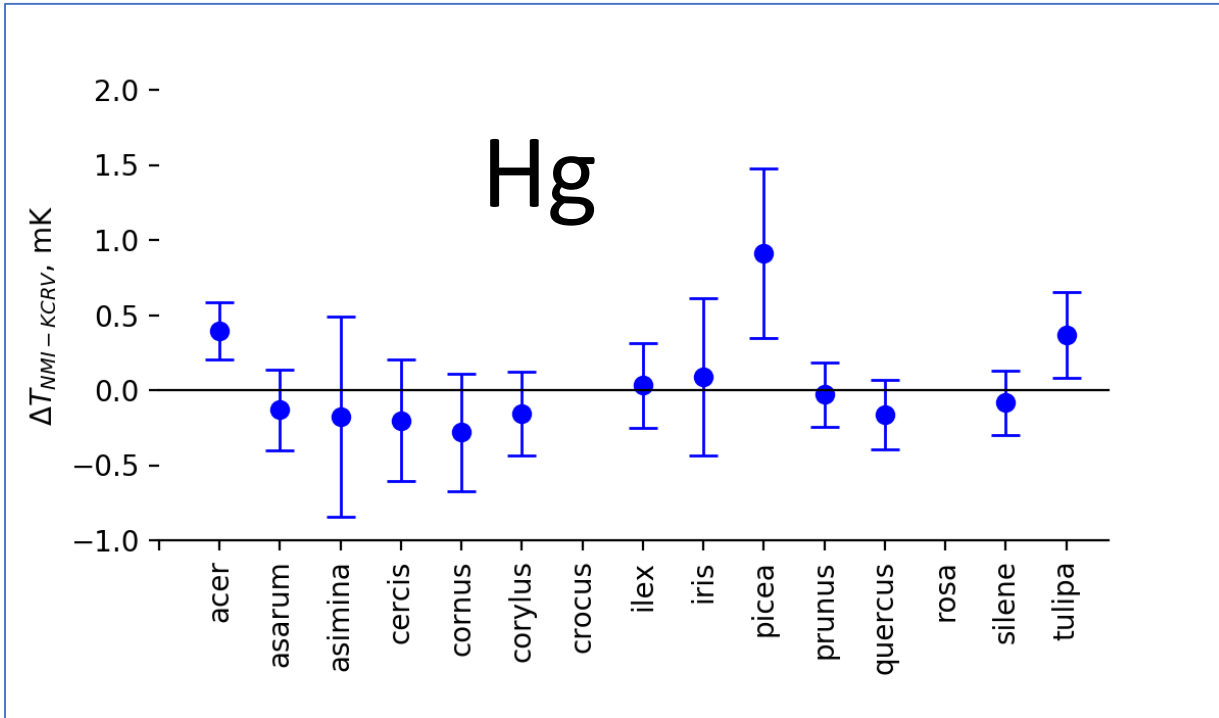

KCRV and results

	KCRV (mK)	u(KCRV) (mK)	$E_n > 1$ (# labs)
Zn	0.04	0.20	5
Sn	0.26	0.14	2
In	0.07	0.08	3
Ga	0.21	0.06	7
Hg	0.37	0.07	3
Ar	0.81	0.14	3

Changes underway to Draft A

1. Two NMIs: unstable SPRT data will be excluded
2. Stabilization procedure at NIST will be documented in Section 3.2 (“Data collection at NIST”)
3. R_0 (TPW) values will be included for final measurement at NIST
4. Some errors of transcription, and some adjustments to uncertainties (determined before draft was unblinded), will be made
5. **Final Draft A to be distributed by pilot by 01 Dec. 2020**