

Key comparisons CCT-K5, CCT-K5.1, APMP.T-K5 and EUROMET.T-K5

MEASURAND : Temperature

NOMINAL TEMPERATURE : $T_{\text{nom}} = 1200 \text{ }^{\circ}\text{C}$

Key comparison CCT-K5

Four Tungsten-strip lamps were used as transfer standards for radiance temperature measurements at specific currents corresponding to each nominal temperature T_{nom} . To shorten the measurement time significantly the set of transfer standards was split in two sets of two lamps for simultaneous comparisons in two loops. The pilot of each loop measured both lamp sets in order to establish a linkage mechanism described on page 19 of the CCT-K5 Final Report.

T_i : temperature value measured by laboratory i

u_i : standard uncertainty of T_i

Lamp S/N C564

Lab <i>i</i>	T_i / °C	u_i / °C
VSL	1201.915	0.12
NMIA	1201.925	0.02
KRISS	1201.915	0.12
NIM	1201.925	0.16
A*STAR	1201.415	0.18
NMIJ	1202.105	0.15
VNIIM	1201.595	0.34

Lamp S/N C681

Lab <i>i</i>	T_i / °C	u_i / °C
VSL	1202.045	0.12
NMIA	1202.095	0.02
KRISS	1202.155	0.12
NIM	1202.315	0.16
A*STAR	1201.245	0.18
NMIJ	1202.255	0.15
VNIIM	1201.585	0.34

Lamp S/N C860

Lab <i>i</i>	T_i / °C	u_i / °C
NPL	1200.191	0.20
NIST	1200.851	0.31
CENAM	1200.561	0.31
LNE-INM	1199.951	0.19
INRIM	1200.671	0.10
PTB	1200.621	0.19

Lamp S/N C864

Lab <i>i</i>	T_i / °C	u_i / °C
NPL	1200.105	0.20
NIST	1200.565	0.31
CENAM	1200.495	0.31
LNE-INM	1200.245	0.19
INRIM	1200.475	0.10
PTB	1200.495	0.19

Key comparison CCT-K5.1

This is a bilateral comparison between the PTB and the NRC.

T_{NRC} : temperature value measured at the NRC

u_{NRC} : standard uncertainty of T_{NRC}

Lamp C598

$$T_{\text{NRC}} = 1200.19 \text{ }^{\circ}\text{C}$$

$$u_{\text{NRC}} = 0.27 \text{ }^{\circ}\text{C}$$

Lamp 644C

$$T_{\text{NRC}} = 1200.33 \text{ }^{\circ}\text{C}$$

$$u_{\text{NRC}} = 0.27 \text{ }^{\circ}\text{C}$$

Key comparison APMP.T-K5

Laboratory individual measurements of APMP.T-K5 participants are given in Appendix B of the APMP.T-K5 Final Report both in tabulated and in graphical forms. There were taken between 1997 and 2000.

Key comparison EUROMET.T-K5

This comparison involved eight participants and was carried out from October 1999 to February 2001.

The two transfer standards were Lamp S/N C564 and Lamp S/N C681 already used in CCT-K5.

The individual laboratory measurements and their uncertainties are given in Tables 5 to 11 of the EUROMET.T-K5 Final Report.

Key comparisons CCT-K5, CCT-K5.1, APMP.T-K5 and EUROMET.T-K5

Key comparison CCT-K5

MEASURAND : Temperature

NOMINAL TEMPERATURE : $T_{\text{nom}} = 1200 \text{ }^{\circ}\text{C}$

The key comparison reference value T_R for each nominal temperature T_{nom} and each lamp k is calculated on the basis of the median of measured radiance temperatures $T_i(k, T_{\text{nom}})$. Its standard uncertainty, $u(T_R)$, is obtained as the standard uncertainty of the median.

Lamp	$T_R / ^{\circ}\text{C}$	$u(T_R) / ^{\circ}\text{C}$
C564	1202.020	0.087
C681	1202.050	0.046
C860	1200.590	0.052
C864	1200.460	0.034

For each temperature T_{nom} the degree of equivalence of laboratory i with respect to the key comparison reference value is given by a pair of terms: D_i and its expanded uncertainty U_i ($k = 2$) both expressed in K. The computation of D_i and U_i is explained in the Addendum to the CCT-K5 Final Report.

For each temperature T_{nom} the pair-wise degree of equivalence between laboratory i and j is given by two terms: D_{ij} and its expanded uncertainty U_{ij} ($k = 2$). The computation of D_{ij} and U_{ij} is also explained in the Addendum of the CCT-K5 Final Report.

Linking key comparison CCT-K5.1 to CCT-K5

The linkage is made through the common participation of PTB in both key comparisons, and is detailed in the CCT-K5 and CCT-K5.1 Linkage Report.

Linking key comparison APMP.T-K5 to CCT-K5

The linkage is made through the common participation of NMIJ, NIM, KRISS and NMIA in both key comparisons, and is detailed in the Addendum to the APMP.T-K5 Final Report.

Linking key comparison EUROMET.T-K5 to CCT-K5

The measurements of the EUROMET.T-K5 participants are directly linked to the key comparison reference value obtained in CCT-K5 as the protocols of the two key comparisons are identical and the transfer standards are the same (see in Chapter VII of the EUROMET.T-K5 Final Report).

Degrees of equivalence relative to the CCT-K5 key comparison reference values are computed for each of the transfer standards. Pair-wise degrees of equivalence inside EUROMET.T-K5 are available in the EUROMET.T-K5 Final Report (Tables 15 to 36).

Key comparisons CCT-K5, CCT-K5.1, APMP.T-K5 and EUROMET.T-K5

MEASURAND : Temperature

NOMINAL TEMPERATURE : $T_{\text{nom}} = 1200 \text{ }^\circ\text{C}$

Degrees of equivalence relative to the CCT-K5 key comparison reference value

Lab*i*

	D_i	U_i
	/ K	
VSL	-0.055	0.262
NPL	-0.377	0.411
NMIA	-0.025	0.122
KRISS	0.000	0.278
NIM	0.085	0.379
A*STAR	-0.705	0.384
NMIJ	0.145	0.320
VNIIM	-0.445	0.686
NIST	0.183	0.632
CENAM	0.003	0.628
LNE-INM	-0.427	0.445
INRIM	0.048	0.222
PTB	0.033	0.220
NRC	0.088	0.696
A*STAR	-0.08	0.60
CMS/TRI	0.06	0.99

Lamp S/N C564

	D_i	U_i
	/ K	
CEM	0.01	0.39
IPQ	-0.07	0.86
UME	-1.57	0.46
MKEH	-1.28	1.79
SMU	-1.34	0.39
SP	-0.69	0.96
MIKES	-0.67	1.27
VSL	0.04	0.30

Lamp S/N C681

	D_i	U_i
	/ K	
CEM	-0.01	0.34
IPQ	-0.31	0.87
UME	-1.68	0.47
MKEH	-1.28	1.94
SMU	-1.07	0.35
SP	-0.74	0.95
MIKES	-0.78	1.34
VSL	-0.11	0.26

Black: participants in CCT-K5

Green: participant in CCT-K5.1

Blue: participants in APMP.T-K5

Orange: participants in EUROMET.T-K5 (measurements with Lamp S/N C564)

Grey: participants in EUROMET.T-K5 (measurements with Lamp S/N C681)

Key comparisons CCT-K5 and CCT-K5.1

MEASURAND : Temperature

NOMINAL TEMPERATURE : $T_{nom} = 1200\text{ °C}$


Matrix of equivalence

Pair-wise degrees of equivalence involving APMP.T-K5 participants are not computed.

Lab _i ↓	Lab _j →		VSL		NPL		NMIA		KRISS		NIM		A*STAR		NMIJ		VNIIM	
	D_i	U_i	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}
	/ K		/ K		/ K		/ K		/ K		/ K		/ K		/ K		/ K	
VSL	-0.055	0.262			0.322	0.478	-0.030	0.244	-0.055	0.343	-0.140	0.421	0.650	0.458	-0.200	0.384	0.390	0.724
NPL	-0.377	0.411	-0.322	0.478			-0.352	0.416	-0.377	0.481	-0.462	0.532	0.328	0.550	-0.522	0.511	0.068	0.795
NMIA	-0.025	0.122	0.030	0.244	0.352	0.416			-0.025	0.246	-0.110	0.340	0.680	0.400	-0.170	0.303	0.420	0.687
KRISS	0.000	0.278	0.055	0.343	0.377	0.481	0.025	0.246			-0.085	0.407	0.705	0.479	-0.145	0.387	0.445	0.732
NIM	0.085	0.379	0.140	0.421	0.462	0.532	0.110	0.340	0.085	0.407			0.790	0.557	-0.060	0.455	0.530	0.778
A*STAR	-0.705	0.384	-0.650	0.458	-0.328	0.550	-0.680	0.400	-0.705	0.479	-0.790	0.557			-0.850	0.496	-0.260	0.773
NMIJ	0.145	0.320	0.200	0.384	0.522	0.511	0.170	0.303	0.145	0.387	0.060	0.455	0.850	0.496			0.590	0.747
VNIIM	-0.445	0.686	-0.390	0.724	-0.068	0.795	-0.420	0.687	-0.445	0.732	-0.530	0.778	0.260	0.773	-0.590	0.747		
NIST	0.183	0.632	0.238	0.674	0.560	0.745	0.208	0.632	0.183	0.676	0.098	0.714	0.888	0.728	0.038	0.698	0.628	0.927
CENAM	0.003	0.628	0.058	0.673	0.380	0.738	0.028	0.631	0.003	0.675	-0.082	0.713	0.708	0.727	-0.142	0.697	0.448	0.926
LNE-INM	-0.427	0.445	-0.372	0.477	-0.050	0.584	-0.402	0.415	-0.427	0.480	-0.512	0.532	0.278	0.550	-0.572	0.510	0.018	0.795
INRIM	0.048	0.222	0.103	0.330	0.425	0.450	0.073	0.231	0.048	0.334	-0.037	0.404	0.753	0.428	-0.097	0.376	0.493	0.716
PTB	0.033	0.220	0.088	0.461	0.410	0.552	0.058	0.397	0.033	0.464	-0.052	0.518	0.738	0.536	-0.112	0.495	0.478	0.785
NRC	0.088	0.696	0.143	0.743	0.465	0.808	0.113	0.706	0.088	0.749	0.003	0.792	0.793	0.795	-0.057	0.766	0.533	0.977

Lab _i ↓	Lab _j →		NIST		CENAM		LNE-INM		INRIM		PTB		NRC	
	D_i	U_i	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}	D_{ij}	U_{ij}
	/ K		/ K		/ K		/ K		/ K		/ K		/ K	
VSL	-0.055	0.262	-0.238	0.674	-0.058	0.673	0.372	0.477	-0.103	0.330	-0.088	0.461	-0.143	0.743
NPL	-0.377	0.411	-0.560	0.745	-0.380	0.738	0.050	0.584	-0.425	0.450	-0.410	0.552	-0.465	0.808
NMIA	-0.025	0.122	-0.208	0.632	-0.028	0.631	0.402	0.415	-0.073	0.231	-0.058	0.397	-0.113	0.706
KRISS	0.000	0.278	-0.183	0.676	-0.003	0.675	0.427	0.480	-0.048	0.334	-0.033	0.464	-0.088	0.749
NIM	0.085	0.379	-0.098	0.714	0.082	0.713	0.512	0.532	0.037	0.404	0.052	0.518	-0.003	0.792
A*STAR	-0.705	0.384	-0.888	0.728	-0.708	0.727	-0.278	0.550	-0.753	0.428	-0.738	0.536	-0.793	0.795
NMIJ	0.145	0.320	-0.038	0.698	0.142	0.697	0.572	0.510	0.097	0.376	0.112	0.495	0.057	0.766
VNIIM	-0.445	0.686	-0.628	0.927	-0.448	0.926	-0.018	0.795	-0.493	0.716	-0.478	0.785	-0.533	0.977
NIST	0.183	0.632			0.180	0.884	0.610	0.783	0.135	0.653	0.150	0.731	0.095	0.940
CENAM	0.003	0.628	-0.180	0.884			0.430	0.749	-0.045	0.654	-0.030	0.728	-0.085	0.937
LNE-INM	-0.427	0.445	-0.610	0.783	-0.430	0.749			-0.475	0.494	-0.460	0.577	-0.515	0.826
INRIM	0.048	0.222	-0.135	0.653	0.045	0.654	0.475	0.494			0.015	0.430	-0.040	0.731
PTB	0.033	0.220	-0.150	0.731	0.030	0.728	0.460	0.577	-0.015	0.430			-0.055	0.730
NRC	0.088	0.696	-0.095	0.940	0.085	0.937	0.515	0.826	0.040	0.731	0.055	0.730		

CCT-K5, CCT-K5.1, APMP.T-K5 and EUROMET.T-K5 Nominal temperature, $T_{\text{nom}} = 1200\text{ °C}$
 Degrees of equivalence, D_i , and expanded uncertainties ($k = 2$) U_i , expressed in K

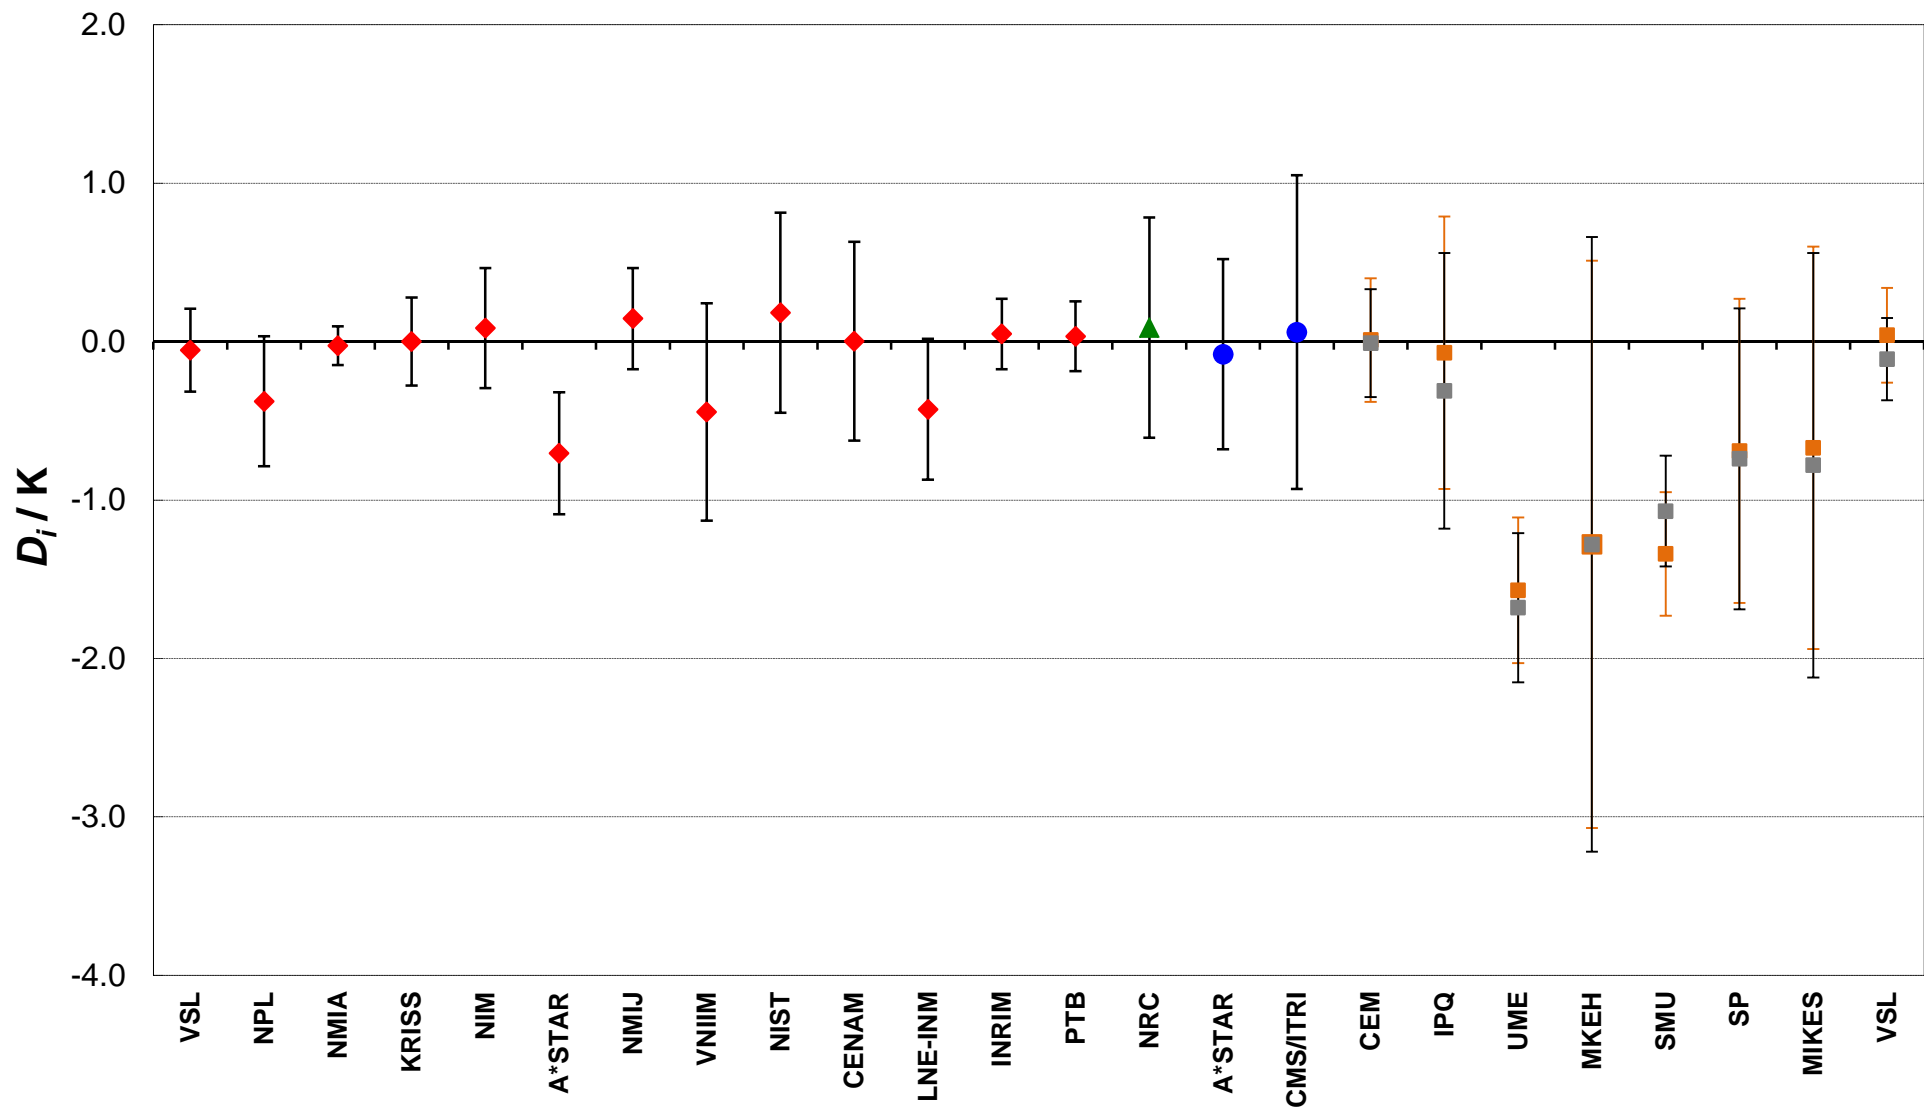

Red diamonds: participants in CCT-K5
 Green triangle: participant in CCT-K5.1
 Blue circles: participants in APMP.T-K5

Orange squares: participants in EUROMET.T-K5 (measurements with Lamp S/N C564)
 Grey squares: participants in EUROMET.T-K5 (measurements with Lamp S/N C681)