

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 1 kHz

$x_i$  adjusted value of the measurement reported by laboratory  $i$  (see on page 13 of the CCEM-K9 Final Report and on page 11 of the EUROMET.EM-K9 Final Report)

$U_i$  expanded uncertainty of  $x_i$  at a 95 % level of confidence

Lab $i$	$x_i$ / ( $\mu\text{V/V}$ )	$U_i$ / ( $\mu\text{V/V}$ )	Date of measurement	Participant in	
				CCEM-K9	EUROMET.EM-K9
LNE	-0.1	12.2	Feb 2000	Yes	Yes
BEV	1.5	10.2	Apr 2000	No	Yes
MIKES	0.6	7.1	May 2000	No	Yes
INETI	6.5	16.2	Jun 2000	No	Yes
AREPA	3.5	11.2	Jul 2000	Yes	Yes
NPL	6.5	12.2	Aug 2000	Yes	Yes
SP	3.5	7.3	Sep 2000	Yes	Yes
IEN	2.2	8.9	Oct 2000	Yes	Yes
CEM	3.5	22.1	Nov 2000	Yes	Yes
PTB	-0.5	8.0	Jan 2001	Yes	Yes
NMi-VSL	-	-	May 2001	Yes	Yes
OMH	-	-	Oct 2001	No	Yes
JV	0.6	18.5	Mar 2002	No	Yes
UME	0.3	18.1	Apr 2002	No	Yes
INTI	-3.1	10.2	Jul 2000	Yes	No
NMIA	-0.2	7.3	Nov 2000	Yes	No
NRC	-0.1	10.2	Mar 2001	Yes	No
VNIIM	2.4	12.8	May 2001	Yes	No
METAS	-1.5	6.3	Aug 2001	Yes	Yes
NIST	5.4	5.9	Jan 2002	Yes	No
NIM	0.1	11.2	May 2002	Yes	No
CMI	-1.1	24.1	Dec 2002	No	Yes

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 1 kHz

The key comparison reference value,  $x_R$ , is computed as the weighted average of the adjusted values obtained by the CCEM-K9 participants. Its expanded uncertainty is  $U_R = 2u_R$ , where  $u_R$  is the standard uncertainty of the weighted average. All adjusted values from CCEM-K9 participants have been taken into account in the calculation, except the value of AREPA, which is traceable to PTB.

$$x_R = 1.4 \mu\text{V/V}, U_R = 2.4 \mu\text{V/V}$$

The degree of equivalence of laboratory  $i$  relative to the key comparison reference value is given by two terms:

$D_i = (x_i - x_R)$  and its expanded uncertainty  $U_i$  at a 95 % level of confidence computed as explained on page 15 of the CCEM-K9 Final Report and on page 12 of the EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The degree of equivalence between two laboratories  $i$  and  $j$  is given by two terms:

$D_{ij} = (D_i - D_j)$  and its expanded uncertainty  $U_{ij}$  at a 95 % level of confidence computed as explained in the Appendices 1 of the CCEM-K9 Final Report and EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The CCEM-K9 Matrix of equivalence is extended with degrees of equivalence between participants in EUROMET.EM-K9.

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 1 kHz

Lab *j* →

Lab *i* ↓

	<i>D<sub>i</sub></i> / (μV/V)		<i>U<sub>i</sub></i> / (μV/V)		LNE		AREPA		NPL		SP		IEN		CEM	
	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)	<i>D<sub>ij</sub></i> / (μV/V)	<i>U<sub>ij</sub></i> / (μV/V)
LNE	-1.5	12.0														
AREPA	2.1	10.9														
NPL	5.1	12.0														
SP	2.1	6.9														
IEN	0.8	8.6														
CEM	2.1	22.0														
PTB	-1.9	7.6														
NMi-VSL	-	-														
INTI	-4.5	9.9														
NMIA	-1.6	6.9														
NRC	-1.5	9.9														
VNIIM	1.0	12.6														
METAS	-2.9	5.8														
NIST	4.0	5.4														
NIM	-1.3	10.9														
BEV	0.1	10.5														
MIKES	-0.8	7.5														
INETI	5.1	16.4														
OMH	-	-														
JV	-0.8	18.7														
UME	-1.1	18.3														
CMI	-2.5	24.2														

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 1 kHz

Lab *j* →

Lab *i* ↓

	Lab <i>i</i>		PTB		NMi-VSL		INTI		NMIA		NRC		VNIIM	
	$D_i$ / (μV/V)	$U_i$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
LNE	-1.5	12.0	0.4	14.6	-	-	3.0	16.0	0.1	14.3	0.0	16.0	-2.5	17.7
AREPA	2.1	10.9	4.0	7.9	-	-	6.6	15.2	3.7	13.4	3.6	15.2	1.1	17.1
NPL	5.1	12.0	7.0	14.6	-	-	9.6	16.0	6.7	14.3	6.6	16.0	4.1	17.7
SP	2.1	6.9	4.0	10.9	-	-	6.6	12.6	3.7	10.4	3.6	12.6	1.1	14.8
IEN	0.8	8.6	2.7	12.0	-	-	5.3	13.6	2.4	11.6	2.3	13.6	-0.2	15.6
CEM	2.1	22.0	4.0	23.6	-	-	6.6	24.4	3.7	23.3	3.6	24.4	1.1	25.6
PTB	-1.9	7.6			-	-	2.6	13.0	-0.3	10.9	-0.4	13.0	-2.9	15.1
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-4.5	9.9	-2.6	13.0	-	-			-2.9	12.6	-3.0	14.5	-5.5	16.4
NMIA	-1.6	6.9	0.3	10.9	-	-	2.9	12.6			-0.1	12.6	-2.6	14.8
NRC	-1.5	9.9	0.4	13.0	-	-	3.0	14.5	0.1	12.6			-2.5	16.4
VNIIM	1.0	12.6	2.9	15.1	-	-	5.5	16.4	2.6	14.8	2.5	16.4		
METAS	-2.9	5.8	-1.0	10.2	-	-	1.6	12.0	-1.3	9.7	-1.4	12.0	-3.9	14.3
NIST	4.0	5.4	5.9	10.0	-	-	8.5	11.8	5.6	9.4	5.5	11.8	3.0	14.1
NIM	-1.3	10.9	0.6	13.8	-	-	3.2	15.2	0.3	13.4	0.2	15.2	-2.3	17.1
BEV	0.1	10.5	2.0	13.0	-	-	-	-	-	-	-	-	-	-
MIKES	-0.8	7.5	1.1	10.7	-	-	-	-	-	-	-	-	-	-
INETI	5.1	16.4	7.0	18.1	-	-	-	-	-	-	-	-	-	-
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	-0.8	18.7	1.1	20.2	-	-	-	-	-	-	-	-	-	-
UME	-1.1	18.3	0.8	19.8	-	-	-	-	-	-	-	-	-	-
CMI	-2.5	24.2	-0.6	25.4	-	-	-	-	-	-	-	-	-	-

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 1 kHz

Lab *j* →

Lab *i* ↓

	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-1.5	12.0
AREPA	2.1	10.9
NPL	5.1	12.0
SP	2.1	6.9
IEN	0.8	8.6
CEM	2.1	22.0
PTB	-1.9	7.6
NMi-VSL	-	-
INTI	-4.5	9.9
NMIA	-1.6	6.9
NRC	-1.5	9.9
VNIIM	1.0	12.6
METAS	-2.9	5.8
NIST	4.0	5.4
NIM	-1.3	10.9

METAS		NIST		NIM		BEV		MIKES		INETI	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
1.4	13.8	-5.5	13.6	-0.2	16.6	-1.6	16.0	-0.7	14.2	-6.6	20.3
5.0	12.9	-1.9	12.7	3.4	15.9	2.0	15.2	2.9	13.3	-3.0	19.7
8.0	13.8	1.1	13.6	6.4	16.6	5.0	16.0	5.9	14.2	0.0	20.3
5.0	9.7	-1.9	9.4	3.4	13.4	2.0	12.6	2.9	10.2	-3.0	17.8
3.7	11.0	-3.2	10.7	2.1	14.4	0.7	13.6	1.6	11.4	-4.3	18.5
5.0	23.0	-1.9	22.9	3.4	24.8	2.0	24.4	2.9	23.3	-3.0	27.5
1.0	10.2	-5.9	10.0	-0.6	13.8	-2.0	13.0	-1.1	10.7	-7.0	18.1
-	-	-	-	-	-	-	-	-	-	-	-
-1.6	12.0	-8.5	11.8	-3.2	15.2	-	-	-	-	-	-
1.3	9.7	-5.6	9.4	-0.3	13.4	-	-	-	-	-	-
1.4	12.0	-5.5	11.8	-0.2	15.2	-	-	-	-	-	-
3.9	14.3	-3.0	14.1	2.3	17.1	-	-	-	-	-	-
		-6.9	8.7	-1.6	12.9	-3.0	12.0	-2.1	9.5	-8.0	17.4
6.9	8.7			5.3	12.7	-	-	-	-	-	-
1.6	12.9	-5.3	12.7			-	-	-	-	-	-

BEV	0.1	10.5
MIKES	-0.8	7.5
INETI	5.1	16.4
OMH	-	-
JV	-0.8	18.7
UME	-1.1	18.3
CMI	-2.5	24.2

3.0	12.0	-	-	-	-			0.9	12.5	-5.0	19.2
2.1	9.5	-	-	-	-	-0.9	12.5			-5.9	17.7
8.0	17.4	-	-	-	-	5.0	19.2	5.9	17.7		
-	-	-	-	-	-	-	-	-	-	-	-
2.1	19.6	-	-	-	-	-0.9	21.2	0.0	19.9	-5.9	24.6
1.8	19.2	-	-	-	-	-1.2	20.8	-0.3	19.5	-6.2	24.3
0.4	25.0	-	-	-	-	-2.6	26.2	-1.7	25.2	-7.6	29.1

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 1 kHz

Lab *j* →

Lab *i* ↓


	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-1.5	12.0
AREPA	2.1	10.9
NPL	5.1	12.0
SP	2.1	6.9
IEN	0.8	8.6
CEM	2.1	22.0
PTB	-1.9	7.6
NMi-VSL	-	-
INTI	-4.5	9.9
NMIA	-1.6	6.9
NRC	-1.5	9.9
VNIIM	1.0	12.6
METAS	-2.9	5.8
NIST	4.0	5.4
NIM	-1.3	10.9

OMH		JV		UME		CMI	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
-	-	-0.7	22.2	-0.4	21.9	1.0	27.1
-	-	2.9	21.7	3.2	21.3	4.6	26.6
-	-	5.9	22.2	6.2	21.9	7.6	27.1
-	-	2.9	19.9	3.2	19.6	4.6	25.2
-	-	1.6	20.6	1.9	20.2	3.3	25.7
-	-	2.9	28.9	3.2	28.6	4.6	32.7
-	-	-1.1	20.2	-0.8	19.8	0.6	25.4
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-2.1	19.6	-1.8	19.2	-0.4	25.0
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-

BEV	0.1	10.5
MIKES	-0.8	7.5
INETI	5.1	16.4
OMH	-	-
JV	-0.8	18.7
UME	-1.1	18.3
CMI	-2.5	24.2

-	-	0.9	21.2	1.2	20.8	2.6	26.2
-	-	0.0	19.9	0.3	19.5	1.7	25.2
-	-	5.9	24.6	6.2	24.3	7.6	29.1
-	-	-	-	-	-	-	-
-	-	-	-	0.3	25.9	1.7	30.4
-	-	-0.3	25.9	-	-	1.4	30.2
-	-	-1.7	30.4	-1.4	30.2	-	-

**CCEM-K9 and EUROMET.EM-K9 AC-DC transfer difference: 200 V, 1 kHz**  
**Degrees of equivalence,  $D_i$ , and expanded uncertainty  $U_i$  (95 % level of confidence)**

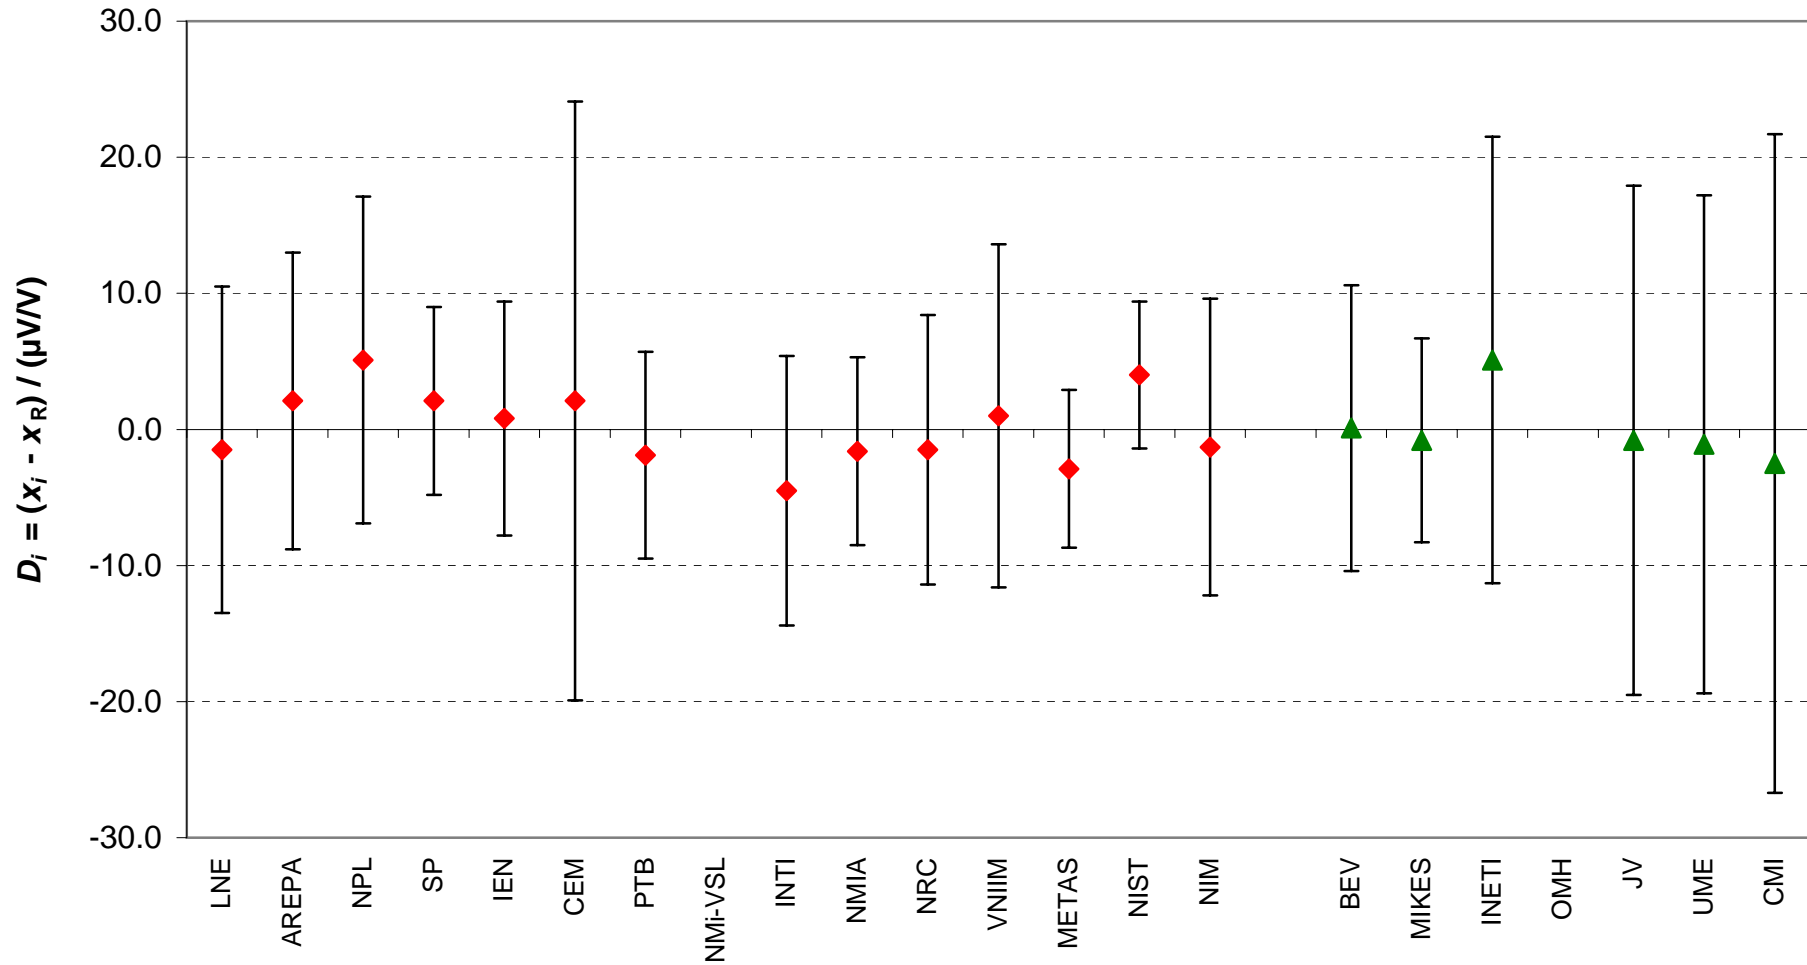

**Red diamonds:** participants in CCEM-K9, **Green triangles:** participants in EUROMET.EM-K9 only

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 10 kHz

$x_i$  adjusted value of the measurement reported by laboratory  $i$  (see on page 13 of the CCEM-K9 Final Report and on page 11 of the EUROMET.EM-K9 Final Report)

$U_i$  expanded uncertainty of  $x_i$  at a 95 % level of confidence

Lab $i$	$x_i$ / ( $\mu\text{V/V}$ )	$U_i$ / ( $\mu\text{V/V}$ )	Date of measurement	Participant in	
				CCEM-K9	EUROMET.EM-K9
LNE	-5.8	13.1	Feb 2000	Yes	Yes
BEV	-0.6	10.2	Apr 2000	No	Yes
MIKES	-1.8	5.9	May 2000	No	Yes
INETI	2.4	16.1	Jun 2000	No	Yes
AREPA	0.4	11.1	Jul 2000	Yes	Yes
NPL	-7.6	12.1	Aug 2000	Yes	Yes
SP	2.4	8.2	Sep 2000	Yes	Yes
IEN	-3.6	9.0	Oct 2000	Yes	Yes
CEM	3.4	22.1	Nov 2000	Yes	Yes
PTB	-3.3	8.0	Jan 2001	Yes	Yes
NMi-VSL	-	-	May 2001	Yes	Yes
OMH	-	-	Oct 2001	No	Yes
JV	-1.5	18.5	Mar 2002	No	Yes
UME	-2.2	18.1	Apr 2002	No	Yes
INTI	-5.2	10.1	Jul 2000	Yes	No
NMIA	-2.2	7.2	Nov 2000	Yes	No
NRC	-3.2	10.1	Mar 2001	Yes	No
VNIIM	-1.3	12.5	May 2001	Yes	No
METAS	-4.4	6.2	Aug 2001	Yes	Yes
NIST	1.0	6.0	Jan 2002	Yes	No
NIM	-5.6	11.1	May 2002	Yes	No
CMI	-10.2	24.1	Dec 2002	No	Yes



## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 10 kHz

The key comparison reference value,  $x_R$ , is computed as the weighted average of the adjusted values obtained by the CCEM-K9 participants. Its expanded uncertainty is  $U_R = 2u_R$ , where  $u_R$  is the standard uncertainty of the weighted average. All adjusted values from CCEM-K9 participants have been taken into account in the calculation, except the value of AREPA, which is traceable to PTB.

$$x_R = -2.5 \mu\text{V/V}, U_R = 2.5 \mu\text{V/V}$$

The degree of equivalence of laboratory  $i$  relative to the key comparison reference value is given by two terms:

$D_i = (x_i - x_R)$  and its expanded uncertainty  $U_i$  at a 95 % level of confidence computed as explained on page 15 of the CCEM-K9 Final Report and on page 12 of the EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The degree of equivalence between two laboratories  $i$  and  $j$  is given by two terms:

$D_{ij} = (D_i - D_j)$  and its expanded uncertainty  $U_{ij}$  at a 95 % level of confidence computed as explained in the Appendices 1 of the CCEM-K9 Final Report and EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The CCEM-K9 Matrix of equivalence is extended with degrees of equivalence between participants in EUROMET.EM-K9.

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 10 kHz

Lab j  $\Rightarrow$

Lab i  $\Downarrow$

	$D_i$ / ( $\mu$ V/V)	$U_i$ / ( $\mu$ V/V)
LNE	-3.3	12.9
AREPA	2.9	10.8
NPL	-5.1	11.8
SP	4.9	7.8
IEN	-1.1	8.6
CEM	5.9	22.0
PTB	-0.8	7.6
NMi-VSL	-	-
INTI	-2.7	9.8
NMIA	0.3	6.8
NRC	-0.7	9.8
VNIIM	1.2	12.2
METAS	-1.9	5.7
NIST	3.5	5.5
NIM	-3.1	10.8

LNE		AREPA		NPL		SP		IEN		CEM	
$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)
		-6.2	17.2	1.8	17.9	-8.2	15.5	-2.2	15.9	-9.2	25.7
6.2	17.2			8.0	16.5	-2.0	13.9	4.0	14.3	-3.0	24.8
-1.8	17.9	-8.0	16.5			-10.0	14.7	-4.0	15.1	-11.0	25.2
8.2	15.5	2.0	13.9	10.0	14.7			6.0	12.2	-1.0	23.6
2.2	15.9	-4.0	14.3	4.0	15.1	-6.0	12.2			-7.0	23.9
9.2	25.7	3.0	24.8	11.0	25.2	1.0	23.6	7.0	23.9		
2.5	15.4	-3.7	7.7	4.3	14.6	-5.7	11.5	0.3	12.1	-6.7	23.6
-	-	-	-	-	-	-	-	-	-	-	-
0.6	16.6	-5.6	15.1	2.4	15.8	-7.6	13.1	-1.6	13.6	-8.6	24.3
3.6	15.0	-2.6	13.3	5.4	14.1	-4.6	11.0	1.4	11.6	-5.6	23.3
2.6	16.6	-3.6	15.1	4.4	15.8	-5.6	13.1	0.4	13.6	-6.6	24.3
4.5	18.2	-1.7	16.8	6.3	17.4	-3.7	15.0	2.3	15.5	-4.7	25.4
1.4	14.5	-4.8	12.8	3.2	13.6	-6.8	10.3	-0.8	11.0	-7.8	23.0
6.8	14.5	0.6	12.7	8.6	13.6	-1.4	10.2	4.6	10.9	-2.4	22.9
0.2	17.2	-6.0	15.7	2.0	16.5	-8.0	13.9	-2.0	14.3	-9.0	24.8

BEV	1.9	10.5
MIKES	0.7	6.4
INETI	4.9	16.3
OMH	-	-
JV	1.0	18.7
UME	0.3	18.3
CMI	-7.7	24.2

5.2	16.7	-1.0	15.1	7.0	15.9	-3.0	13.1	3.0	13.7	-4.0	24.4
4.0	14.4	-2.2	12.6	5.8	13.5	-4.2	10.2	1.8	10.8	-5.2	22.9
8.2	20.8	2.0	19.6	10.0	20.2	0.0	18.1	6.0	18.5	-1.0	27.4
-	-	-	-	-	-	-	-	-	-	-	-
4.3	22.7	-1.9	21.6	6.1	22.2	-3.9	20.3	2.1	20.6	-4.9	28.9
3.6	22.4	-2.6	21.3	5.4	21.8	-4.6	19.9	1.4	20.3	-5.6	28.6
-4.4	27.5	-10.6	26.6	-2.6	27.0	-12.6	25.5	-6.6	25.8	-13.6	32.7

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 10 kHz

Lab *j* →

Lab *i* ↓

	Lab <i>i</i>		PTB		NMi-VSL		INTI		NMIA		NRC		VNIIM	
	$D_i$ / (μV/V)	$U_i$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
LNE	-3.3	12.9	-2.5	15.4	-	-	-0.6	16.6	-3.6	15.0	-2.6	16.6	-4.5	18.2
AREPA	2.9	10.8	3.7	7.7	-	-	5.6	15.1	2.6	13.3	3.6	15.1	1.7	16.8
NPL	-5.1	11.8	-4.3	14.6	-	-	-2.4	15.8	-5.4	14.1	-4.4	15.8	-6.3	17.4
SP	4.9	7.8	5.7	11.5	-	-	7.6	13.1	4.6	11.0	5.6	13.1	3.7	15.0
IEN	-1.1	8.6	-0.3	12.1	-	-	1.6	13.6	-1.4	11.6	-0.4	13.6	-2.3	15.5
CEM	5.9	22.0	6.7	23.6	-	-	8.6	24.3	5.6	23.3	6.6	24.3	4.7	25.4
PTB	-0.8	7.6	-	-	-	-	1.9	12.9	-1.1	10.8	-0.1	12.9	-2.0	14.9
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-2.7	9.8	-1.9	12.9	-	-	-	-	-3.0	12.5	-2.0	14.3	-3.9	16.1
NMIA	0.3	6.8	1.1	10.8	-	-	3.0	12.5	-	-	1.0	12.5	-0.9	14.5
NRC	-0.7	9.8	0.1	12.9	-	-	2.0	14.3	-1.0	12.5	-	-	-1.9	16.1
VNIIM	1.2	12.2	2.0	14.9	-	-	3.9	16.1	0.9	14.5	1.9	16.1	-	-
METAS	-1.9	5.7	-1.1	10.2	-	-	0.8	11.9	-2.2	9.6	-1.2	11.9	-3.1	14.0
NIST	3.5	5.5	4.3	10.0	-	-	6.2	11.8	3.2	9.4	4.2	11.8	2.3	13.9
NIM	-3.1	10.8	-2.3	13.7	-	-	-0.4	15.1	-3.4	13.3	-2.4	15.1	-4.3	16.8
BEV	1.9	10.5	2.7	13.0	-	-	-	-	-	-	-	-	-	-
MIKES	0.7	6.4	1.5	10.0	-	-	-	-	-	-	-	-	-	-
INETI	4.9	16.3	5.7	18.0	-	-	-	-	-	-	-	-	-	-
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	1.0	18.7	1.8	20.2	-	-	-	-	-	-	-	-	-	-
UME	0.3	18.3	1.1	19.8	-	-	-	-	-	-	-	-	-	-
CMI	-7.7	24.2	-6.9	25.4	-	-	-	-	-	-	-	-	-	-

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 10 kHz

Lab *j* →

Lab *i* ↓

	Lab <i>i</i>		METAS		NIST		NIM		BEV		MIKES		INETI	
	$D_i$ / (μV/V)	$U_i$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
LNE	-3.3	12.9	-1.4	14.5	-6.8	14.5	-0.2	17.2	-5.2	16.7	-4.0	14.4	-8.2	20.8
AREPA	2.9	10.8	4.8	12.8	-0.6	12.7	6.0	15.7	1.0	15.1	2.2	12.6	-2.0	19.6
NPL	-5.1	11.8	-3.2	13.6	-8.6	13.6	-2.0	16.5	-7.0	15.9	-5.8	13.5	-10.0	20.2
SP	4.9	7.8	6.8	10.3	1.4	10.2	8.0	13.9	3.0	13.1	4.2	10.2	0.0	18.1
IEN	-1.1	8.6	0.8	11.0	-4.6	10.9	2.0	14.3	-3.0	13.7	-1.8	10.8	-6.0	18.5
CEM	5.9	22.0	7.8	23.0	2.4	22.9	9.0	24.8	4.0	24.4	5.2	22.9	1.0	27.4
PTB	-0.8	7.6	1.1	10.2	-4.3	10.0	2.3	13.7	-2.7	13.0	-1.5	10.0	-5.7	18.0
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-2.7	9.8	-0.8	11.9	-6.2	11.8	0.4	15.1	-	-	-	-	-	-
NMIA	0.3	6.8	2.2	9.6	-3.2	9.4	3.4	13.3	-	-	-	-	-	-
NRC	-0.7	9.8	1.2	11.9	-4.2	11.8	2.4	15.1	-	-	-	-	-	-
VNIIM	1.2	12.2	3.1	14.0	-2.3	13.9	4.3	16.8	-	-	-	-	-	-
METAS	-1.9	5.7			-5.4	8.7	1.2	12.8	-3.8	12.0	-2.6	8.6	-6.8	17.3
NIST	3.5	5.5	5.4	8.7			6.6	12.7	-	-	-	-	-	-
NIM	-3.1	10.8	-1.2	12.8	-6.6	12.7			-	-	-	-	-	-
BEV	1.9	10.5	3.8	12.0	-	-	-	-			1.2	11.8	-3.0	19.1
MIKES	0.7	6.4	2.6	8.6	-	-	-	-	-1.2	11.8			-4.2	17.2
INETI	4.9	16.3	6.8	17.3	-	-	-	-	3.0	19.1	4.2	17.2		
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	1.0	18.7	2.9	19.6	-	-	-	-	-0.9	21.2	0.3	19.5	-3.9	24.6
UME	0.3	18.3	2.2	19.2	-	-	-	-	-1.6	20.8	-0.4	19.1	-4.6	24.3
CMI	-7.7	24.2	-5.8	24.9	-	-	-	-	-9.6	26.2	-8.4	24.9	-12.6	29.0

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 10 kHz

Lab *j* →

Lab *i* ↓


	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-3.3	12.9
AREPA	2.9	10.8
NPL	-5.1	11.8
SP	4.9	7.8
IEN	-1.1	8.6
CEM	5.9	22.0
PTB	-0.8	7.6
NMi-VSL	-	-
INTI	-2.7	9.8
NMIA	0.3	6.8
NRC	-0.7	9.8
VNIIM	1.2	12.2
METAS	-1.9	5.7
NIST	3.5	5.5
NIM	-3.1	10.8

OMH		JV		UME		CMI	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
-	-	-4.3	22.7	-3.6	22.4	4.4	27.5
-	-	1.9	21.6	2.6	21.3	10.6	26.6
-	-	-6.1	22.2	-5.4	21.8	2.6	27.0
-	-	3.9	20.3	4.6	19.9	12.6	25.5
-	-	-2.1	20.6	-1.4	20.3	6.6	25.8
-	-	4.9	28.9	5.6	28.6	13.6	32.7
-	-	-1.8	20.2	-1.1	19.8	6.9	25.4
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-2.9	19.6	-2.2	19.2	5.8	24.9
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-

BEV	1.9	10.5
MIKES	0.7	6.4
INETI	4.9	16.3
OMH	-	-
JV	1.0	18.7
UME	0.3	18.3
CMI	-7.7	24.2

-	-	0.9	21.2	1.6	20.8	9.6	26.2
-	-	-0.3	19.5	0.4	19.1	8.4	24.9
-	-	3.9	24.6	4.6	24.3	12.6	29.0
-	-	-	-	-	-	-	-
-	-	-	-	0.7	25.9	8.7	30.4
-	-	-0.7	25.9	-	-	8.0	30.2
-	-	-8.7	30.4	-8.0	30.2	-	-

**CCEM-K9 and EUROMET.EM-K9 AC-DC transfer difference: 200 V, 10 kHz**  
**Degrees of equivalence,  $D_i$  and expanded uncertainty  $U_i$  (95 % level of confidence)**

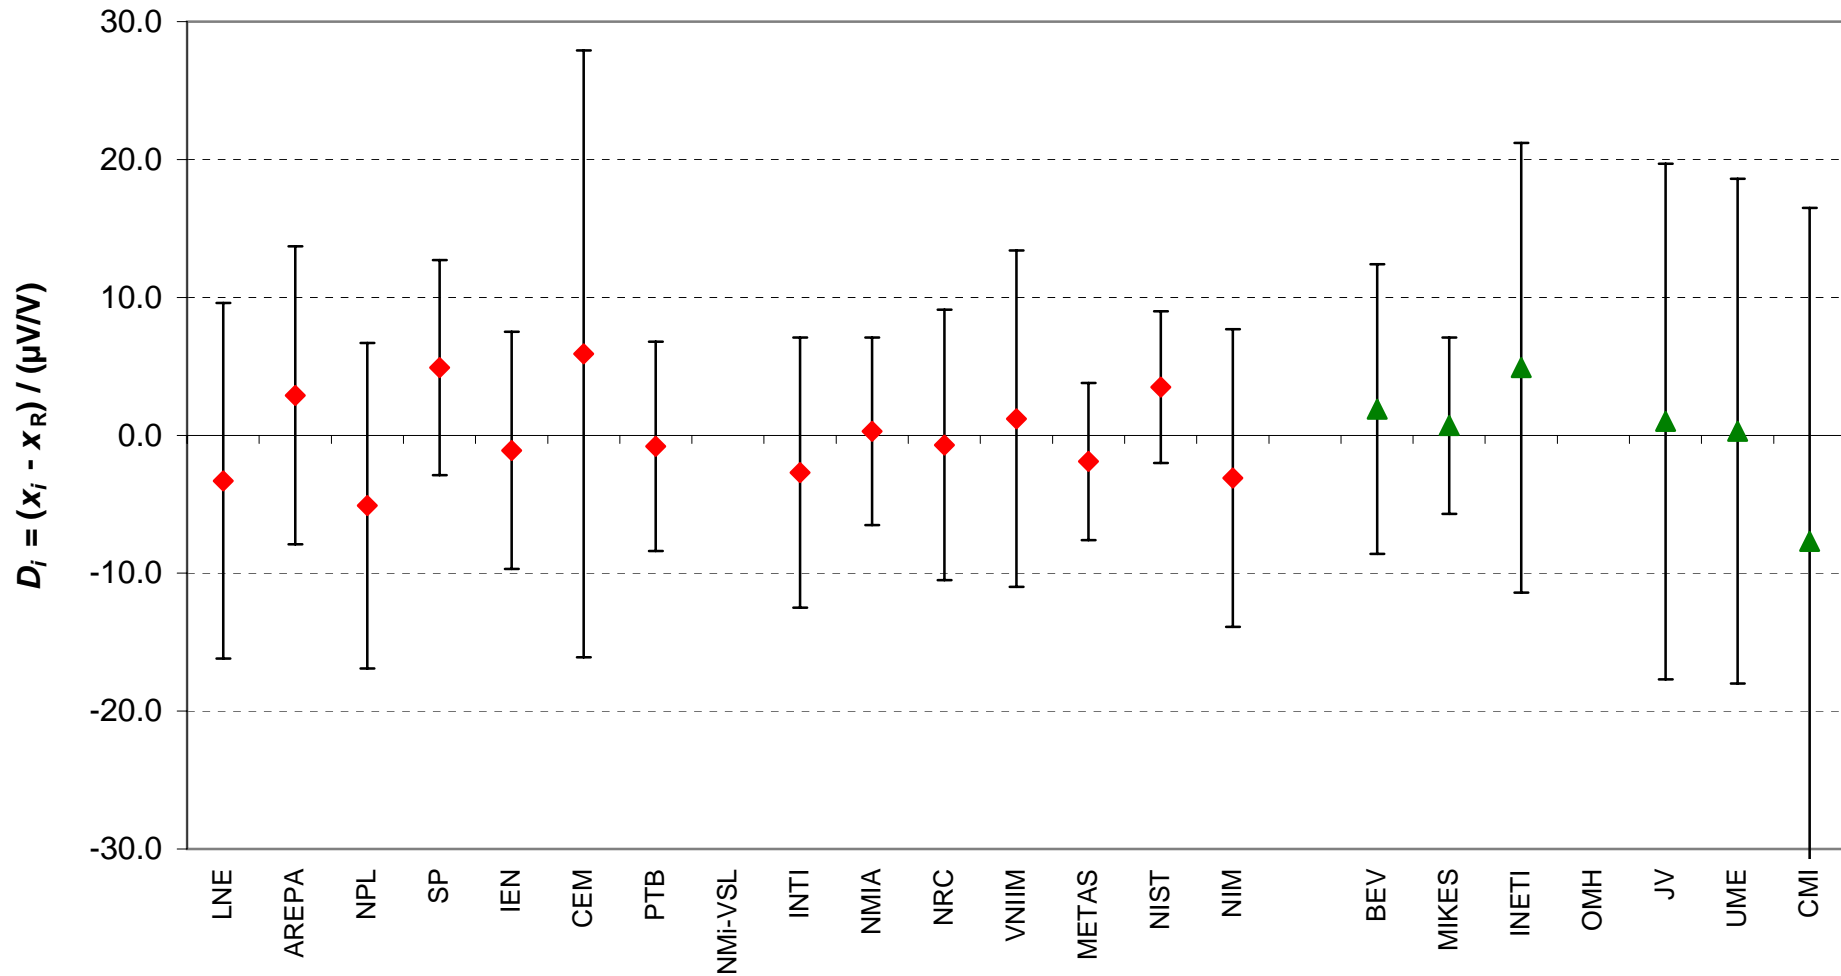

**Red diamonds:** participants in CCEM-K9, **Green triangles:** participants in EUROMET.EM-K9 only

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 20 kHz

$x_i$  adjusted value of the measurement reported by laboratory  $i$  (see on page 13 of the CCEM-K9 Final Report and on page 11 of the EUROMET.EM-K9 Final Report)

$U_i$  expanded uncertainty of  $x_i$  at a 95 % level of confidence

Lab $i$	$x_i$ / ( $\mu\text{V/V}$ )	$U_i$ / ( $\mu\text{V/V}$ )	Date of measurement	Participant in	
				CCEM-K9	EUROMET.EM-K9
LNE	-7.7	13.1	Feb 2000	Yes	Yes
BEV	-3.6	12.1	Apr 2000	No	Yes
MIKES	-4.7	6.6	May 2000	No	Yes
INETI	-1.6	18.0	Jun 2000	No	Yes
AREPA	-4.6	11.1	Jul 2000	Yes	Yes
NPL	-9.6	14.1	Aug 2000	Yes	Yes
SP	-1.6	9.1	Sep 2000	Yes	Yes
IEN	-11.0	12.9	Oct 2000	Yes	Yes
CEM	-0.6	22.0	Nov 2000	Yes	Yes
PTB	-7.3	8.0	Jan 2001	Yes	Yes
NMi-VSL	-	-	May 2001	Yes	Yes
OMH	-	-	Oct 2001	No	Yes
JV	-5.1	20.0	Mar 2002	No	Yes
UME	-8.1	24.0	Apr 2002	No	Yes
INTI	-8.3	12.1	Jul 2000	Yes	No
NMIA	-6.3	8.1	Nov 2000	Yes	No
NRC	-4.3	10.1	Mar 2001	Yes	No
VNIIM	-3.3	20.2	May 2001	Yes	No
METAS	-7.5	6.1	Aug 2001	Yes	Yes
NIST	-2.5	6.1	Jan 2002	Yes	No
NIM	-8.8	11.1	May 2002	Yes	No
CMI	-10.3	28.0	Dec 2002	No	Yes

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 20 kHz

The key comparison reference value,  $x_R$ , is computed as the weighted average of the adjusted values obtained by the CCEM-K9 participants. Its expanded uncertainty is  $U_R = 2u_R$ , where  $u_R$  is the standard uncertainty of the weighted average. All adjusted values from CCEM-K9 participants have been taken into account in the calculation, except the value of AREPA, which is traceable to PTB.

$$x_R = -5.9 \mu\text{V/V}, U_R = 2.6 \mu\text{V/V}$$

The degree of equivalence of laboratory  $i$  relative to the key comparison reference value is given by two terms:

$D_i = (x_i - x_R)$  and its expanded uncertainty  $U_i$  at a 95 % level of confidence computed as explained on page 15 of the CCEM-K9 Final Report and on page 12 of the EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The degree of equivalence between two laboratories  $i$  and  $j$  is given by two terms:

$D_{ij} = (D_i - D_j)$  and its expanded uncertainty  $U_{ij}$  at a 95 % level of confidence computed as explained in the Appendices 1 of the CCEM-K9 Final Report and EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The CCEM-K9 Matrix of equivalence is extended with degrees of equivalence between participants in EUROMET.EM-K9.



Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 20 kHz

Lab *j* →

Lab *i* ↓

	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-1.8	12.8
AREPA	1.3	10.8
NPL	-3.7	13.9
SP	4.3	8.7
IEN	-5.1	12.6
CEM	5.3	21.8
PTB	-1.4	7.6
NMi-VSL	-	-
INTI	-2.4	11.8
NMIA	-0.4	7.7
NRC	1.6	9.8
VNIIM	2.6	20.0
METAS	-1.6	5.5
NIST	3.4	5.5
NIM	-2.9	10.8

LNE		AREPA		NPL		SP		IEN		CEM	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
		-3.1	17.2	1.9	19.3	-6.1	16.0	3.3	18.4	-7.1	25.7
3.1	17.2			5.0	18.0	-3.0	14.4	6.4	17.1	-4.0	24.7
-1.9	19.3	-5.0	18.0			-8.0	16.8	1.4	19.2	-9.0	26.2
6.1	16.0	3.0	14.4	8.0	16.8			9.4	15.8	-1.0	23.9
-3.3	18.4	-6.4	17.1	-1.4	19.2	-9.4	15.8			-10.4	25.6
7.1	25.7	4.0	24.7	9.0	26.2	1.0	23.9	10.4	25.6		
0.4	15.4	-2.7	7.7	2.3	16.3	-5.7	12.2	3.7	15.2	-6.7	23.5
-	-	-	-	-	-	-	-	-	-	-	-
-0.6	17.9	-3.7	16.5	1.3	18.6	-6.7	15.2	2.7	17.7	-7.7	25.2
1.4	15.5	-1.7	13.8	3.3	16.3	-4.7	12.2	4.7	15.3	-5.7	23.5
3.4	16.6	0.3	15.1	5.3	17.4	-2.7	13.6	6.7	16.4	-3.7	24.3
4.4	24.1	1.3	23.1	6.3	24.7	-1.7	22.2	7.7	24.0	-2.7	29.9
0.2	14.5	-2.9	12.7	2.1	15.4	-5.9	11.0	3.5	14.3	-6.9	22.9
5.2	14.5	2.1	12.7	7.1	15.4	-0.9	11.0	8.5	14.3	-1.9	22.9
-1.1	17.2	-4.2	15.7	0.8	18.0	-7.2	14.4	2.2	17.1	-8.2	24.7

BEV	2.3	12.4
MIKES	1.2	7.1
INETI	4.3	18.2
OMH	-	-
JV	0.8	20.2
UME	-2.2	24.1
CMI	-4.4	28.1

4.1	17.9	1.0	16.5	6.0	18.6	-2.0	15.2	7.4	17.7	-3.0	25.2
3.0	14.7	-0.1	13.0	4.9	15.6	-3.1	11.3	6.3	14.5	-4.1	23.0
6.1	22.3	3.0	21.2	8.0	22.9	0.0	20.2	9.4	22.2	-1.0	28.5
-	-	-	-	-	-	-	-	-	-	-	-
2.6	24.0	-0.5	22.9	4.5	24.5	-3.5	22.0	5.9	23.8	-4.5	29.8
-0.4	27.4	-3.5	26.5	1.5	27.9	-6.5	25.7	2.9	27.3	-7.5	32.6
-2.6	31.0	-5.7	30.2	-0.7	31.4	-8.7	29.5	0.7	30.9	-9.7	35.7

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 20 kHz

Lab *j* →

Lab *i* ↓

	Lab <i>i</i>		PTB		NMi-VSL		INTI		NMIA		NRC		VNIIM	
	$D_i$ / (μV/V)	$U_i$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
LNE	-1.8	12.8	-0.4	15.4	-	-	0.6	17.9	-1.4	15.5	-3.4	16.6	-4.4	24.1
AREPA	1.3	10.8	2.7	7.7	-	-	3.7	16.5	1.7	13.8	-0.3	15.1	-1.3	23.1
NPL	-3.7	13.9	-2.3	16.3	-	-	-1.3	18.6	-3.3	16.3	-5.3	17.4	-6.3	24.7
SP	4.3	8.7	5.7	12.2	-	-	6.7	15.2	4.7	12.2	2.7	13.6	1.7	22.2
IEN	-5.1	12.6	-3.7	15.2	-	-	-2.7	17.7	-4.7	15.3	-6.7	16.4	-7.7	24.0
CEM	5.3	21.8	6.7	23.5	-	-	7.7	25.2	5.7	23.5	3.7	24.3	2.7	29.9
PTB	-1.4	7.6	-	-	1.0	14.6	-1.0	11.4	-3.0	12.9	-4.0	21.8	-	-
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-2.4	11.8	-1.0	14.6	-	-	-	-	-2.0	14.6	-4.0	15.8	-5.0	23.6
NMIA	-0.4	7.7	1.0	11.4	-	-	2.0	14.6	-	-	-2.0	13.0	-3.0	21.8
NRC	1.6	9.8	3.0	12.9	-	-	4.0	15.8	2.0	13.0	-	-	-1.0	22.6
VNIIM	2.6	20.0	4.0	21.8	-	-	5.0	23.6	3.0	21.8	1.0	22.6	-	-
METAS	-1.6	5.5	-0.2	10.1	-	-	0.8	13.6	-1.2	10.2	-3.2	11.8	-4.2	21.2
NIST	3.4	5.5	4.8	10.1	-	-	5.8	13.6	3.8	10.2	1.8	11.8	0.8	21.2
NIM	-2.9	10.8	-1.5	13.7	-	-	-0.5	16.5	-2.5	13.8	-4.5	15.1	-5.5	23.1
BEV	2.3	12.4	3.7	14.6	-	-	-	-	-	-	-	-	-	-
MIKES	1.2	7.1	2.6	10.4	-	-	-	-	-	-	-	-	-	-
INETI	4.3	18.2	5.7	19.7	-	-	-	-	-	-	-	-	-	-
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	0.8	20.2	2.2	21.6	-	-	-	-	-	-	-	-	-	-
UME	-2.2	24.1	-0.8	25.3	-	-	-	-	-	-	-	-	-	-
CMI	-4.4	28.1	-3.0	29.2	-	-	-	-	-	-	-	-	-	-

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 20 kHz

Lab *j* →

Lab *i* ↓

	Lab <i>i</i>		METAS		NIST		NIM		BEV		MIKES		INETI	
	$D_i$ / (μV/V)	$U_i$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
LNE	-1.8	12.8	-0.2	14.5	-5.2	14.5	1.1	17.2	-4.1	17.9	-3.0	14.7	-6.1	22.3
AREPA	1.3	10.8	2.9	12.7	-2.1	12.7	4.2	15.7	-1.0	16.5	0.1	13.0	-3.0	21.2
NPL	-3.7	13.9	-2.1	15.4	-7.1	15.4	-0.8	18.0	-6.0	18.6	-4.9	15.6	-8.0	22.9
SP	4.3	8.7	5.9	11.0	0.9	11.0	7.2	14.4	2.0	15.2	3.1	11.3	0.0	20.2
IEN	-5.1	12.6	-3.5	14.3	-8.5	14.3	-2.2	17.1	-7.4	17.7	-6.3	14.5	-9.4	22.2
CEM	5.3	21.8	6.9	22.9	1.9	22.9	8.2	24.7	3.0	25.2	4.1	23.0	1.0	28.5
PTB	-1.4	7.6	0.2	10.1	-4.8	10.1	1.5	13.7	-3.7	14.6	-2.6	10.4	-5.7	19.7
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-2.4	11.8	-0.8	13.6	-5.8	13.6	0.5	16.5	-	-	-	-	-	-
NMIA	-0.4	7.7	1.2	10.2	-3.8	10.2	2.5	13.8	-	-	-	-	-	-
NRC	1.6	9.8	3.2	11.8	-1.8	11.8	4.5	15.1	-	-	-	-	-	-
VNIIM	2.6	20.0	4.2	21.2	-0.8	21.2	5.5	23.1	-	-	-	-	-	-
METAS	-1.6	5.5			-5.0	8.7	1.3	12.7	-3.9	13.6	-2.8	9.0	-5.9	19.1
NIST	3.4	5.5	5.0	8.7			6.3	12.7	-	-	-	-	-	-
NIM	-2.9	10.8	-1.3	12.7	-6.3	12.7			-	-	-	-	-	-
BEV	2.3	12.4	3.9	13.6	-	-	-	-			1.1	13.8	-2.0	21.7
MIKES	1.2	7.1	2.8	9.0	-	-	-	-	-1.1	13.8			-3.1	19.2
INETI	4.3	18.2	5.9	19.1	-	-	-	-	2.0	21.7	3.1	19.2		
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	0.8	20.2	2.4	21.0	-	-	-	-	-1.5	23.4	-0.4	21.1	-3.5	27.0
UME	-2.2	24.1	-0.6	24.8	-	-	-	-	-4.5	26.9	-3.4	24.9	-6.5	30.0
CMI	-4.4	28.1	-2.8	28.7	-	-	-	-	-6.7	30.6	-5.6	28.8	-8.7	33.3

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 20 kHz

Lab *j* →

Lab *i* ↓


	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-1.8	12.8
AREPA	1.3	10.8
NPL	-3.7	13.9
SP	4.3	8.7
IEN	-5.1	12.6
CEM	5.3	21.8
PTB	-1.4	7.6
NMi-VSL	-	-
INTI	-2.4	11.8
NMIA	-0.4	7.7
NRC	1.6	9.8
VNIIM	2.6	20.0
METAS	-1.6	5.5
NIST	3.4	5.5
NIM	-2.9	10.8

OMH		JV		UME		CMI	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
-	-	-2.6	24.0	0.4	27.4	2.6	31.0
-	-	0.5	22.9	3.5	26.5	5.7	30.2
-	-	-4.5	24.5	-1.5	27.9	0.7	31.4
-	-	3.5	22.0	6.5	25.7	8.7	29.5
-	-	-5.9	23.8	-2.9	27.3	-0.7	30.9
-	-	4.5	29.8	7.5	32.6	9.7	35.7
-	-	-2.2	21.6	0.8	25.3	3.0	29.2
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-2.4	21.0	0.6	24.8	2.8	28.7
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-

BEV	2.3	12.4
MIKES	1.2	7.1
INETI	4.3	18.2
OMH	-	-
JV	0.8	20.2
UME	-2.2	24.1
CMI	-4.4	28.1

-	-	1.5	23.4	4.5	26.9	6.7	30.6
-	-	0.4	21.1	3.4	24.9	5.6	28.8
-	-	3.5	27.0	6.5	30.0	8.7	33.3
-	-	-	-	-	-	-	-
-	-	-	-	3.0	31.3	5.2	34.5
-	-	-3.0	31.3	-	-	2.2	36.9
-	-	-5.2	34.5	-2.2	36.9	-	-

**CCEM-K9 and EUROMET.EM-K9 AC-DC transfer difference: 200 V, 20 kHz**  
**Degrees of equivalence,  $D_i$  and expanded uncertainty  $U_i$  (95 % level of confidence)**

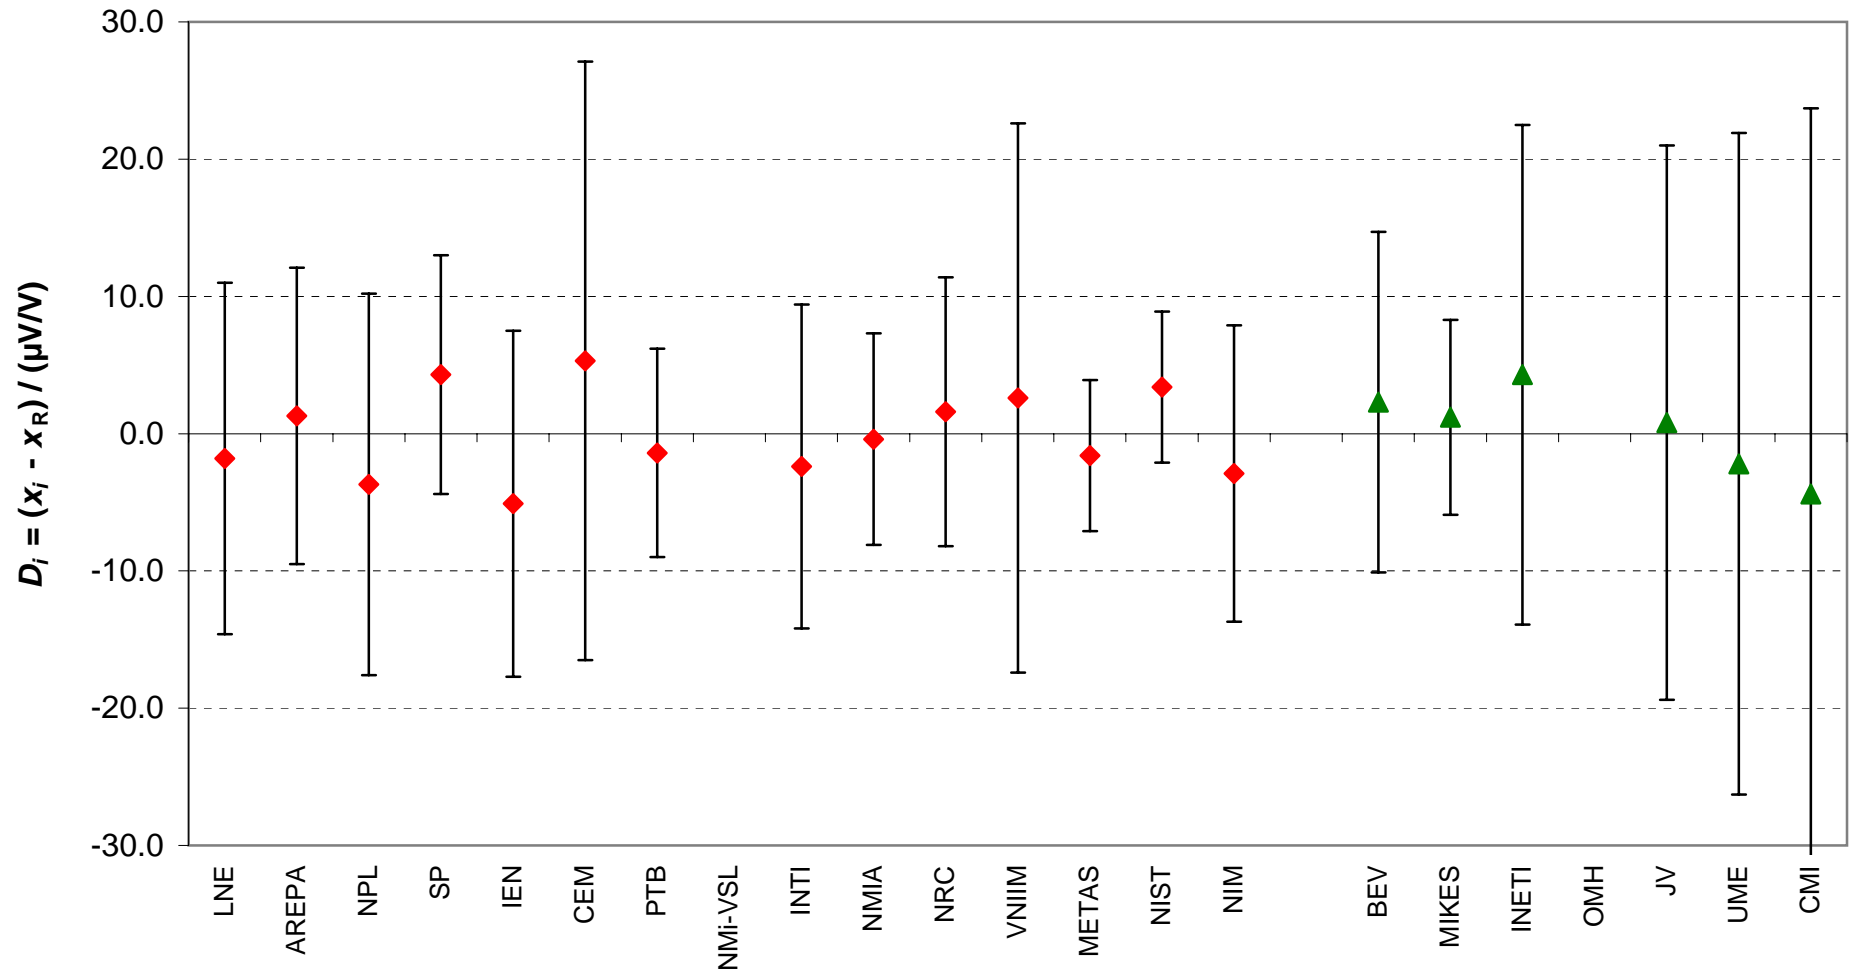

**Red diamonds:** participants in CCEM-K9, **Green triangles:** participants in EUROMET.EM-K9 only

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 50 kHz

$x_i$  adjusted value of the measurement reported by laboratory  $i$  (see on page 13 of the CCEM-K9 Final Report and on page 11 of the EUROMET.EM-K9 Final Report)

$U_i$  expanded uncertainty of  $x_i$  at a 95 % level of confidence

Lab $i$	$x_i$ / ( $\mu\text{V/V}$ )	$U_i$ / ( $\mu\text{V/V}$ )	Date of measurement	Participant in	
				CCEM-K9	EUROMET.EM-K9
LNE	-28.2	16.2	Feb 2000	Yes	Yes
BEV	-19.1	16.2	Apr 2000	No	Yes
MIKES	-20.2	7.1	May 2000	No	Yes
INETI	-16.1	20.1	Jun 2000	No	Yes
AREPA	-23.1	11.2	Jul 2000	Yes	Yes
NPL	-23.1	16.2	Aug 2000	Yes	Yes
SP	-18.1	13.2	Sep 2000	Yes	Yes
IEN	-31.8	18.3	Oct 2000	Yes	Yes
CEM	-19.1	24.1	Nov 2000	Yes	Yes
PTB	-22.7	10.0	Jan 2001	Yes	Yes
NMi-VSL	-	-	May 2001	Yes	Yes
OMH	-	-	Oct 2001	No	Yes
JV	-19.3	26.1	Mar 2002	No	Yes
UME	-21.3	30.1	Apr 2002	No	Yes
INTI	-23.7	16.1	Jul 2000	Yes	No
NMIA	-19.7	11.2	Nov 2000	Yes	No
NRC	-16.7	14.1	Mar 2001	Yes	No
VNIIM	-14.1	30.3	May 2001	Yes	No
METAS	-22.8	9.2	Aug 2001	Yes	Yes
NIST	-20.3	8.1	Jan 2002	Yes	No
NIM	-24.4	12.4	May 2002	Yes	No
CMI	-26.7	36.1	Dec 2002	No	Yes

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 50 kHz

The key comparison reference value,  $x_R$ , is computed as the weighted average of the adjusted values obtained by the CCEM-K9 participants. Its expanded uncertainty is  $U_R = 2u_R$ , where  $u_R$  is the standard uncertainty of the weighted average. All adjusted values from CCEM-K9 participants have been taken into account in the calculation, except the value of AREPA, which is traceable to PTB.

$$x_R = -21.9 \mu\text{V/V}, U_R = 3.5 \mu\text{V/V}$$

The degree of equivalence of laboratory  $i$  relative to the key comparison reference value is given by two terms:

$D_i = (x_i - x_R)$  and its expanded uncertainty  $U_i$  at a 95 % level of confidence computed as explained on page 15 of the CCEM-K9 Final Report and on page 12 of the EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The degree of equivalence between two laboratories  $i$  and  $j$  is given by two terms:

$D_{ij} = (D_i - D_j)$  and its expanded uncertainty  $U_{ij}$  at a 95 % level of confidence computed as explained in the Appendices 1 of the CCEM-K9 Final Report and EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The CCEM-K9 Matrix of equivalence is extended with degrees of equivalence between participants in EUROMET.EM-K9.

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 50 kHz

Lab *j* →

Lab *i* ↓

	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-6.3	15.8
AREPA	-1.2	10.6
NPL	-1.2	15.8
SP	3.8	12.7
IEN	-9.9	18.0
CEM	2.8	23.8
PTB	-0.8	9.4
NMi-VSL	-	-
INTI	-1.8	15.7
NMIA	2.2	10.6
NRC	5.2	13.7
VNIIM	7.8	30.1
METAS	-0.9	8.5
NIST	1.6	7.3
NIM	-2.5	11.9

LNE		AREPA		NPL		SP		IEN		CEM	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
		-5.1	19.7	-5.1	23.0	-10.1	20.9	3.6	24.5	-9.1	29.1
5.1	19.7			0.0	19.7	-5.0	17.4	8.7	21.5	-4.0	26.6
5.1	23.0	0.0	19.7			-5.0	20.9	8.7	24.5	-4.0	29.1
10.1	20.9	5.0	17.4	5.0	20.9			13.7	22.6	1.0	27.5
-3.6	24.5	-8.7	21.5	-8.7	24.5	-13.7	22.6			-12.7	30.3
9.1	29.1	4.0	26.6	4.0	29.1	-1.0	27.5	12.7	30.3		
5.5	19.1	0.4	5.1	0.4	19.1	-4.6	16.6	9.1	20.9	-3.6	26.1
-	-	-	-	-	-	-	-	-	-	-	-
4.5	22.9	-0.6	19.7	-0.6	22.9	-5.6	20.9	8.1	24.4	-4.6	29.0
8.5	19.7	3.4	15.9	3.4	19.7	-1.6	17.4	12.1	21.5	-0.6	26.6
11.5	21.5	6.4	18.1	6.4	21.5	1.4	19.4	15.1	23.2	2.4	28.0
14.1	34.4	9.0	32.4	9.0	34.4	4.0	33.1	17.7	35.4	5.0	38.8
5.4	18.7	0.3	14.5	0.3	18.7	-4.7	16.1	9.0	20.5	-3.7	25.8
7.9	18.2	2.8	13.9	2.8	18.2	-2.2	15.5	11.5	20.1	-1.2	25.5
3.8	20.5	-1.3	16.8	-1.3	20.5	-6.3	18.2	7.4	22.2	-5.3	27.2

BEV	2.8	16.6
MIKES	1.7	7.9
INETI	5.8	20.4
OMH	-	-
JV	2.6	26.3
UME	0.6	30.3
CMI	-4.8	36.3

9.1	23.0	4.0	19.7	4.0	23.0	-1.0	20.9	12.7	24.5	0.0	29.1
8.0	17.7	2.9	13.3	2.9	17.7	-2.1	15.0	11.6	19.7	-1.1	25.2
12.1	25.9	7.0	23.1	7.0	25.9	2.0	24.1	15.7	27.2	3.0	31.4
-	-	-	-	-	-	-	-	-	-	-	-
8.9	30.8	3.8	28.5	3.8	30.8	-1.2	29.3	12.5	31.9	-0.2	35.6
6.9	34.2	1.8	32.2	1.8	34.2	-3.2	32.9	10.5	35.3	-2.2	38.6
1.5	39.6	-3.6	37.8	-3.6	39.6	-8.6	38.5	5.1	40.5	-7.6	43.5



Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 50 kHz

Lab j  $\Rightarrow$

Lab i  $\Downarrow$

	Lab i		PTB		NMi-VSL		INTI		NMIA		NRC		VNIIM	
	$D_i$ / ( $\mu$ V/V)	$U_i$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)	$D_{ij}$ / ( $\mu$ V/V)	$U_{ij}$ / ( $\mu$ V/V)
LNE	-6.3	15.8	-5.5	19.1	-	-	-4.5	22.9	-8.5	19.7	-11.5	21.5	-14.1	34.4
AREPA	-1.2	10.6	-0.4	5.1	-	-	0.6	19.7	-3.4	15.9	-6.4	18.1	-9.0	32.4
NPL	-1.2	15.8	-0.4	19.1	-	-	0.6	22.9	-3.4	19.7	-6.4	21.5	-9.0	34.4
SP	3.8	12.7	4.6	16.6	-	-	5.6	20.9	1.6	17.4	-1.4	19.4	-4.0	33.1
IEN	-9.9	18.0	-9.1	20.9	-	-	-8.1	24.4	-12.1	21.5	-15.1	23.2	-17.7	35.4
CEM	2.8	23.8	3.6	26.1	-	-	4.6	29.0	0.6	26.6	-2.4	28.0	-5.0	38.8
PTB	-0.8	9.4	-	-	-	-	1.0	19.0	-3.0	15.1	-6.0	17.3	-8.6	32.0
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-1.8	15.7	-1.0	19.0	-	-	-	-	-4.0	19.7	-7.0	21.5	-9.6	34.4
NMIA	2.2	10.6	3.0	15.1	-	-	4.0	19.7	-	-	-3.0	18.1	-5.6	32.4
NRC	5.2	13.7	6.0	17.3	-	-	7.0	21.5	3.0	18.1	-	-	-2.6	33.5
VNIIM	7.8	30.1	8.6	32.0	-	-	9.6	34.4	5.6	32.4	2.6	33.5	-	-
METAS	-0.9	8.5	-0.1	13.6	-	-	0.9	18.6	-3.1	14.5	-6.1	16.9	-8.7	31.7
NIST	1.6	7.3	2.4	12.9	-	-	3.4	18.1	-0.6	13.9	-3.6	16.3	-6.2	31.4
NIM	-2.5	11.9	-1.7	16.0	-	-	-0.7	20.4	-4.7	16.8	-7.7	18.8	-10.3	32.8
BEV	2.8	16.6	3.6	19.1	-	-	-	-	-	-	-	-	-	-
MIKES	1.7	7.9	2.5	12.3	-	-	-	-	-	-	-	-	-	-
INETI	5.8	20.4	6.6	22.5	-	-	-	-	-	-	-	-	-	-
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	2.6	26.3	3.4	28.0	-	-	-	-	-	-	-	-	-	-
UME	0.6	30.3	1.4	31.8	-	-	-	-	-	-	-	-	-	-
CMI	-4.8	36.3	-4.0	37.5	-	-	-	-	-	-	-	-	-	-

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 50 kHz

Lab *j* →

Lab *i* ↓

	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-6.3	15.8
AREPA	-1.2	10.6
NPL	-1.2	15.8
SP	3.8	12.7
IEN	-9.9	18.0
CEM	2.8	23.8
PTB	-0.8	9.4
NMi-VSL	-	-
INTI	-1.8	15.7
NMIA	2.2	10.6
NRC	5.2	13.7
VNIIM	7.8	30.1
METAS	-0.9	8.5
NIST	1.6	7.3
NIM	-2.5	11.9

METAS		NIST		NIM		BEV		MIKES		INETI	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
-5.4	18.7	-7.9	18.2	-3.8	20.5	-9.1	23.0	-8.0	17.7	-12.1	25.9
-0.3	14.5	-2.8	13.9	1.3	16.8	-4.0	19.7	-2.9	13.3	-7.0	23.1
-0.3	18.7	-2.8	18.2	1.3	20.5	-4.0	23.0	-2.9	17.7	-7.0	25.9
4.7	16.1	2.2	15.5	6.3	18.2	1.0	20.9	2.1	15.0	-2.0	24.1
-9.0	20.5	-11.5	20.1	-7.4	22.2	-12.7	24.5	-11.6	19.7	-15.7	27.2
3.7	25.8	1.2	25.5	5.3	27.2	0.0	29.1	1.1	25.2	-3.0	31.4
0.1	13.6	-2.4	12.9	1.7	16.0	-3.6	19.1	-2.5	12.3	-6.6	22.5
-	-	-	-	-	-	-	-	-	-	-	-
-0.9	18.6	-3.4	18.1	0.7	20.4	-	-	-	-	-	-
3.1	14.5	0.6	13.9	4.7	16.8	-	-	-	-	-	-
6.1	16.9	3.6	16.3	7.7	18.8	-	-	-	-	-	-
8.7	31.7	6.2	31.4	10.3	32.8	-	-	-	-	-	-
		-2.5	12.3	1.6	15.5	-3.7	18.7	-2.6	11.7	-6.7	22.2
2.5	12.3			4.1	14.9	-	-	-	-	-	-
-1.6	15.5	-4.1	14.9			-	-	-	-	-	-

BEV	2.8	16.6
MIKES	1.7	7.9
INETI	5.8	20.4
OMH	-	-
JV	2.6	26.3
UME	0.6	30.3
CMI	-4.8	36.3

3.7	18.7	-	-	-	-			1.1	17.7	-3.0	25.9
2.6	11.7	-	-	-	-	-1.1	17.7			-4.1	21.4
6.7	22.2	-	-	-	-	3.0	25.9	4.1	21.4		
-	-	-	-	-	-	-	-	-	-	-	-
3.5	27.7	-	-	-	-	-0.2	30.8	0.9	27.1	-3.2	33.0
1.5	31.5	-	-	-	-	-2.2	34.2	-1.1	31.0	-5.2	36.2
-3.9	37.3	-	-	-	-	-7.6	39.6	-6.5	36.8	-10.6	41.4

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 50 kHz

Lab *j* →

Lab *i* ↓


	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-6.3	15.8
AREPA	-1.2	10.6
NPL	-1.2	15.8
SP	3.8	12.7
IEN	-9.9	18.0
CEM	2.8	23.8
PTB	-0.8	9.4
NMi-VSL	-	-
INTI	-1.8	15.7
NMIA	2.2	10.6
NRC	5.2	13.7
VNIIM	7.8	30.1
METAS	-0.9	8.5
NIST	1.6	7.3
NIM	-2.5	11.9

OMH		JV		UME		CMI	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
-	-	-8.9	30.8	-6.9	34.2	-1.5	39.6
-	-	-3.8	28.5	-1.8	32.2	3.6	37.8
-	-	-3.8	30.8	-1.8	34.2	3.6	39.6
-	-	1.2	29.3	3.2	32.9	8.6	38.5
-	-	-12.5	31.9	-10.5	35.3	-5.1	40.5
-	-	0.2	35.6	2.2	38.6	7.6	43.5
-	-	-3.4	28.0	-1.4	31.8	4.0	37.5
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-3.5	27.7	-1.5	31.5	3.9	37.3
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-

BEV	2.8	16.6
MIKES	1.7	7.9
INETI	5.8	20.4
OMH	-	-
JV	2.6	26.3
UME	0.6	30.3
CMI	-4.8	36.3

-	-	0.2	30.8	2.2	34.2	7.6	39.6
-	-	-0.9	27.1	1.1	31.0	6.5	36.8
-	-	3.2	33.0	5.2	36.2	10.6	41.4
-	-	-	-	-	-	-	-
-	-	-	-	2.0	39.9	7.4	44.6
-	-	-2.0	39.9	-	-	5.4	47.1
-	-	-7.4	44.6	-5.4	47.1	-	-

**CCEM-K9 and EUROMET.EM-K9 AC-DC transfer difference: 200 V, 50 kHz**  
**Degrees of equivalence,  $D_i$  and expanded uncertainty  $U_i$  (95 % level of confidence)**

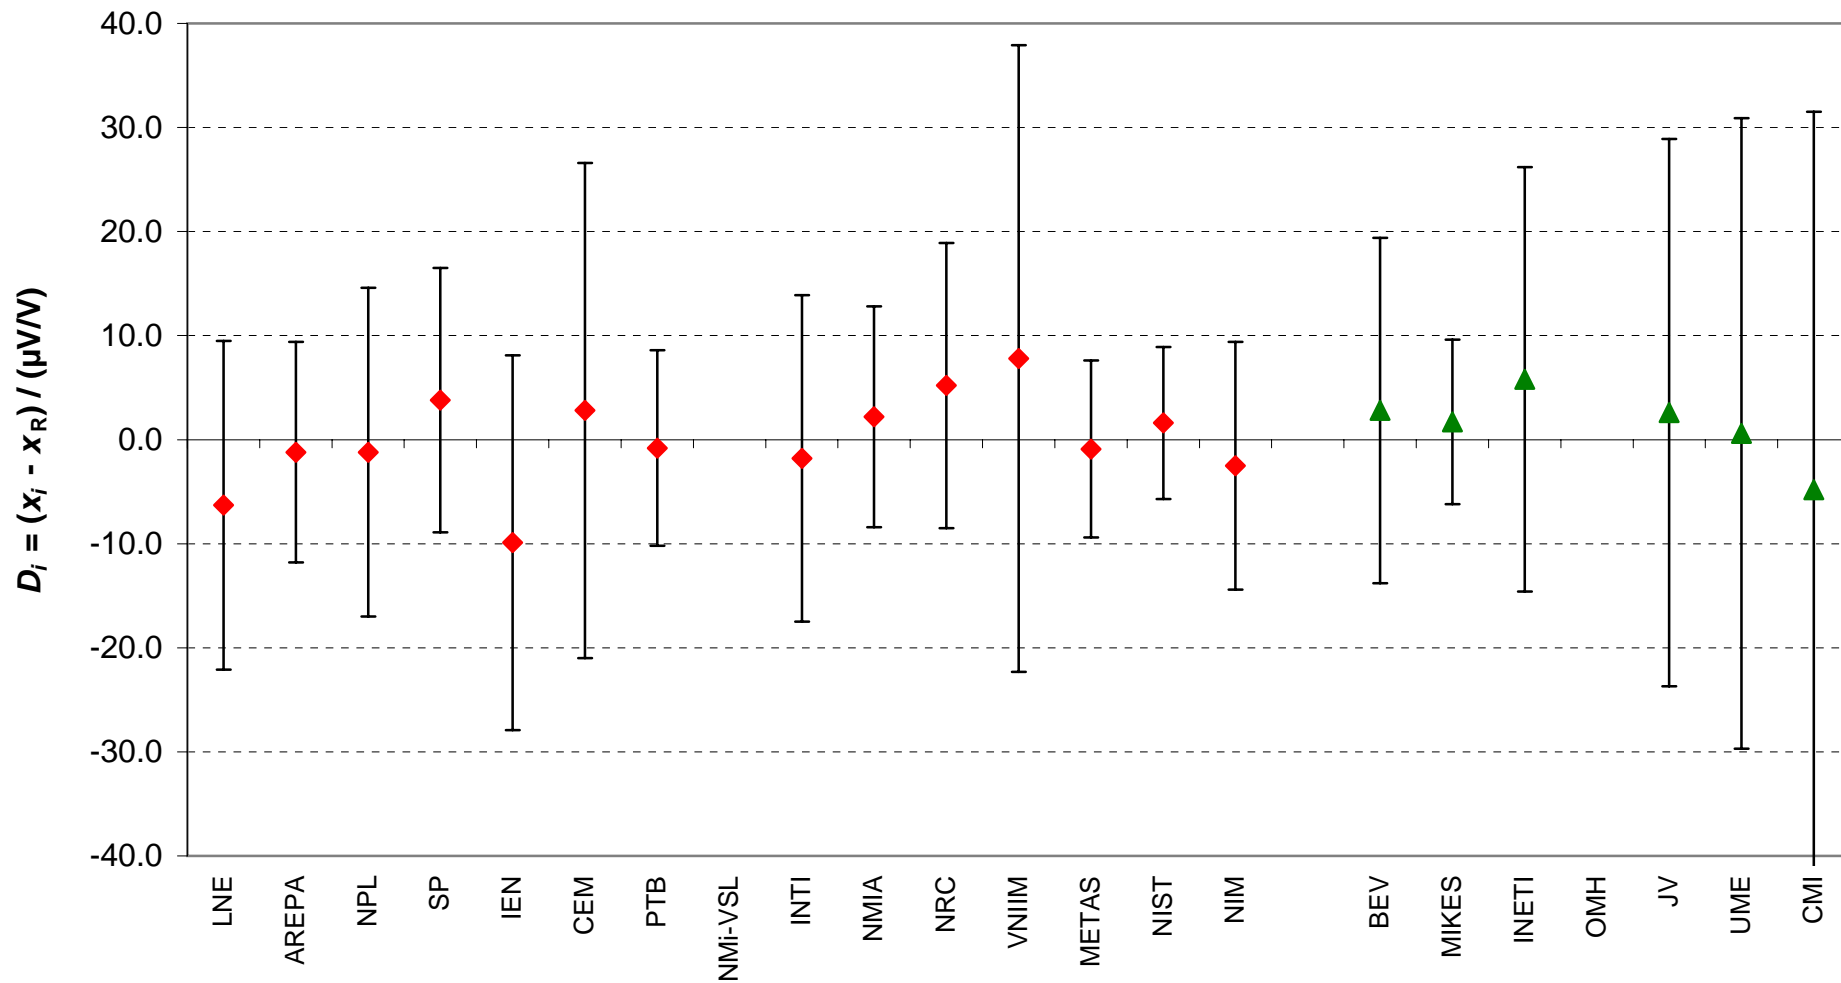

**Red diamonds:** participants in CCEM-K9, **Green triangles:** participants in EUROMET.EM-K9 only

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 100 kHz

$x_i$  adjusted value of the measurement reported by laboratory  $i$  (see on page 13 of the CCEM-K9 Final Report and on page 11 of the EUROMET.EM-K9 Final Report)

$U_i$  expanded uncertainty of  $x_i$  at a 95 % level of confidence

Lab $i$	$x_i$ / ( $\mu\text{V/V}$ )	$U_i$ / ( $\mu\text{V/V}$ )	Date of measurement	Participant in	
				CCEM-K9	EUROMET.EM-K9
LNE	-70.7	16.2	Feb 2000	Yes	Yes
BEV	-52.2	21.1	Apr 2000	No	Yes
MIKES	-54.5	8.5	May 2000	No	Yes
INETI	-49.2	30.1	Jun 2000	No	Yes
AREPA	-66.2	26.1	Jul 2000	Yes	Yes
NPL	-61.2	20.1	Aug 2000	Yes	Yes
SP	-49.2	19.2	Sep 2000	Yes	Yes
IEN	-71.5	42.5	Oct 2000	Yes	Yes
CEM	-54.2	28.9	Nov 2000	Yes	Yes
PTB	-61.9	22.0	Jan 2001	Yes	Yes
NMi-VSL	-	-	May 2001	Yes	Yes
OMH	-	-	Oct 2001	No	Yes
JV	-48.6	36.1	Mar 2002	No	Yes
UME	-59.3	44.1	Apr 2002	No	Yes
INTI	-61.3	24.1	Jul 2000	Yes	No
NMIA	-53.3	18.1	Nov 2000	Yes	No
NRC	-56.3	22.7	Mar 2001	Yes	No
VNIIM	-61.0	40.5	May 2001	Yes	No
METAS	-60.3	24.1	Aug 2001	Yes	Yes
NIST	-58.5	11.0	Jan 2002	Yes	No
NIM	-65.9	13.4	May 2002	Yes	No
CMI	-63.3	60.0	Dec 2002	No	Yes

## Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 100 kHz

The key comparison reference value,  $x_R$ , is computed as the weighted average of the adjusted values obtained by the CCEM-K9 participants. Its expanded uncertainty is  $U_R = 2u_R$ , where  $u_R$  is the standard uncertainty of the weighted average. All adjusted values from CCEM-K9 participants have been taken into account in the calculation, except the value of AREPA, which is traceable to PTB.

$$x_R = -60.4 \mu\text{V/V}, U_R = 5.3 \mu\text{V/V}$$

The degree of equivalence of laboratory  $i$  relative to the key comparison reference value is given by two terms:

$D_i = (x_i - x_R)$  and its expanded uncertainty  $U_i$  at a 95 % level of confidence computed as explained on page 15 of the CCEM-K9 Final Report and on page 12 of the EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The degree of equivalence between two laboratories  $i$  and  $j$  is given by two terms:

$D_{ij} = (D_i - D_j)$  and its expanded uncertainty  $U_{ij}$  at a 95 % level of confidence computed as explained in the Appendices 1 of the CCEM-K9 Final Report and EUROMET.EM-K9 Final Report, both expressed in  $\mu\text{V/V}$ .

The CCEM-K9 Matrix of equivalence is extended with degrees of equivalence between participants in EUROMET.EM-K9.

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 100 kHz

Lab *j* →

Lab *i* ↓

	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-10.3	15.3
AREPA	-5.8	25.6
NPL	-0.8	19.4
SP	11.2	18.5
IEN	-11.1	42.2
CEM	6.2	28.4
PTB	-1.5	21.4
NMi-VSL	-	-
INTI	-0.9	23.5
NMIA	7.1	17.3
NRC	4.1	22.1
VNIIM	-0.6	40.2
METAS	0.1	23.5
NIST	1.9	9.6
NIM	-5.5	12.3

LNE		AREPA		NPL		SP		IEN		CEM	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
		-4.5	30.8	-9.5	25.9	-21.5	25.2	0.8	45.5	-16.5	33.2
4.5	30.8			-5.0	33.0	-17.0	32.5	5.3	49.9	-12.0	39.0
9.5	25.9	5.0	33.0			-12.0	27.8	10.3	47.1	-7.0	35.3
21.5	25.2	17.0	32.5	12.0	27.8			22.3	46.7	5.0	34.7
-0.8	45.5	-5.3	49.9	-10.3	47.1	-22.3	46.7			-17.3	51.4
16.5	33.2	12.0	39.0	7.0	35.3	-5.0	34.7	17.3	51.4		
8.8	27.4	4.3	14.1	-0.7	29.8	-12.7	29.2	9.6	47.9	-7.7	36.4
-	-	-	-	-	-	-	-	-	-	-	-
9.4	29.1	4.9	35.6	-0.1	31.4	-12.1	30.9	10.2	48.9	-7.1	37.7
17.4	24.3	12.9	31.8	7.9	27.1	-4.1	26.4	18.2	46.2	0.9	34.2
14.4	27.9	9.9	34.6	4.9	30.4	-7.1	29.8	15.2	48.2	-2.1	36.8
9.7	43.7	5.2	48.2	0.2	45.3	-11.8	44.9	10.5	58.8	-6.8	49.8
10.4	29.1	5.9	35.6	0.9	31.4	-11.1	30.9	11.2	48.9	-6.1	37.7
12.2	19.6	7.7	28.4	2.7	23.0	-9.3	22.2	13.0	44.0	-4.3	31.0
4.8	21.1	0.3	29.4	-4.7	24.2	-16.7	23.5	5.6	44.6	-11.7	31.9

BEV	8.2	21.8
MIKES	5.9	10.0
INETI	11.2	30.6
OMH	-	-
JV	11.8	36.5
UME	1.1	44.4
CMI	-2.9	60.2

18.5	26.7	14.0	33.6	9.0	29.2	-3.0	28.6	19.3	47.5	2.0	35.8
16.2	18.3	11.7	27.5	6.7	21.9	-5.3	21.0	17.0	43.4	-0.3	30.2
21.5	34.2	17.0	39.9	12.0	36.2	0.0	35.8	22.3	52.1	5.0	41.8
-	-	-	-	-	-	-	-	-	-	-	-
22.1	39.6	17.6	44.6	12.6	41.4	0.6	40.9	22.9	55.8	5.6	46.3
11.4	47.0	6.9	51.3	1.9	48.5	-10.1	48.1	12.2	61.3	-5.1	52.8
7.4	62.2	2.9	65.5	-2.1	63.3	-14.1	63.0	8.2	73.6	-9.1	66.6

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 100 kHz

Lab *j* →

Lab *i* ↓

	Lab <i>i</i>		PTB		NMi-VSL		INTI		NMIA		NRC		VNIIM	
	$D_i$ / (μV/V)	$U_i$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
LNE	-10.3	15.3	-8.8	27.4	-	-	-9.4	29.1	-17.4	24.3	-14.4	27.9	-9.7	43.7
AREPA	-5.8	25.6	-4.3	14.1	-	-	-4.9	35.6	-12.9	31.8	-9.9	34.6	-5.2	48.2
NPL	-0.8	19.4	0.7	29.8	-	-	0.1	31.4	-7.9	27.1	-4.9	30.4	-0.2	45.3
SP	11.2	18.5	12.7	29.2	-	-	12.1	30.9	4.1	26.4	7.1	29.8	11.8	44.9
IEN	-11.1	42.2	-9.6	47.9	-	-	-10.2	48.9	-18.2	46.2	-15.2	48.2	-10.5	58.8
CEM	6.2	28.4	7.7	36.4	-	-	7.1	37.7	-0.9	34.2	2.1	36.8	6.8	49.8
PTB	-1.5	21.4	-	-	-	-	-0.6	32.7	-8.6	28.5	-5.6	31.7	-0.9	46.1
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-0.9	23.5	0.6	32.7	-	-	-	-	-8.0	30.2	-5.0	33.2	-0.3	47.2
NMIA	7.1	17.3	8.6	28.5	-	-	8.0	30.2	-	-	3.0	29.1	7.7	44.4
NRC	4.1	22.1	5.6	31.7	-	-	5.0	33.2	-3.0	29.1	-	-	4.7	46.5
VNIIM	-0.6	40.2	0.9	46.1	-	-	0.3	47.2	-7.7	44.4	-4.7	46.5	-	-
METAS	0.1	23.5	1.6	32.7	-	-	1.0	34.1	-7.0	30.2	-4.0	33.2	0.7	47.2
NIST	1.9	9.6	3.4	24.6	-	-	2.8	26.5	-5.2	21.2	-2.2	25.3	2.5	42.0
NIM	-5.5	12.3	-4.0	25.8	-	-	-4.6	27.6	-12.6	22.6	-9.6	26.4	-4.9	42.7
BEV	8.2	21.8	9.7	30.5	-	-	-	-	-	-	-	-	-	-
MIKES	5.9	10.0	7.4	23.6	-	-	-	-	-	-	-	-	-	-
INETI	11.2	30.6	12.7	37.3	-	-	-	-	-	-	-	-	-	-
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	11.8	36.5	13.3	42.3	-	-	-	-	-	-	-	-	-	-
UME	1.1	44.4	2.6	49.3	-	-	-	-	-	-	-	-	-	-
CMI	-2.9	60.2	-1.4	64.0	-	-	-	-	-	-	-	-	-	-



Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 100 kHz

Lab *j* →

Lab *i* ↓

	Lab <i>i</i>		METAS		NIST		NIM		BEV		MIKES		INETI	
	$D_i$ / (μV/V)	$U_i$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
LNE	-10.3	15.3	-10.4	29.1	-12.2	19.6	-4.8	21.1	-18.5	26.7	-16.2	18.3	-21.5	34.2
AREPA	-5.8	25.6	-5.9	35.6	-7.7	28.4	-0.3	29.4	-14.0	33.6	-11.7	27.5	-17.0	39.9
NPL	-0.8	19.4	-0.9	31.4	-2.7	23.0	4.7	24.2	-9.0	29.2	-6.7	21.9	-12.0	36.2
SP	11.2	18.5	11.1	30.9	9.3	22.2	16.7	23.5	3.0	28.6	5.3	21.0	0.0	35.8
IEN	-11.1	42.2	-11.2	48.9	-13.0	44.0	-5.6	44.6	-19.3	47.5	-17.0	43.4	-22.3	52.1
CEM	6.2	28.4	6.1	37.7	4.3	31.0	11.7	31.9	-2.0	35.8	0.3	30.2	-5.0	41.8
PTB	-1.5	21.4	-1.6	32.7	-3.4	24.6	4.0	25.8	-9.7	30.5	-7.4	23.6	-12.7	37.3
NMi-VSL	-	-	-	-	-	-	-	-	-	-	-	-	-	-
INTI	-0.9	23.5	-1.0	34.1	-2.8	26.5	4.6	27.6	-	-	-	-	-	-
NMIA	7.1	17.3	7.0	30.2	5.2	21.2	12.6	22.6	-	-	-	-	-	-
NRC	4.1	22.1	4.0	33.2	2.2	25.3	9.6	26.4	-	-	-	-	-	-
VNIIM	-0.6	40.2	-0.7	47.2	-2.5	42.0	4.9	42.7	-	-	-	-	-	-
METAS	0.1	23.5			-1.8	26.5	5.6	27.6	-8.1	32.1	-5.8	25.6	-11.1	38.6
NIST	1.9	9.6	1.8	26.5			7.4	17.4	-	-	-	-	-	-
NIM	-5.5	12.3	-5.6	27.6	-7.4	17.4			-	-	-	-	-	-
BEV	8.2	21.8	8.1	32.1	-	-	-	-			2.3	22.8	-3.0	36.8
MIKES	5.9	10.0	5.8	25.6	-	-	-	-	-2.3	22.8			-5.3	31.3
INETI	11.2	30.6	11.1	38.6	-	-	-	-	3.0	36.8	5.3	31.3		
OMH	-	-	-	-	-	-	-	-	-	-	-	-	-	-
JV	11.8	36.5	11.7	43.5	-	-	-	-	3.6	41.9	5.9	37.1	0.6	47.1
UME	1.1	44.4	1.0	50.3	-	-	-	-	-7.1	48.9	-4.8	45.0	-10.1	53.4
CMI	-2.9	60.2	-3.0	64.7	-	-	-	-	-11.1	63.7	-8.8	60.6	-14.1	67.2

Key comparisons CCEM-K9 and EUROMET.EM-K9

MEASURAND : AC-DC transfer difference

VOLTAGE : 200 V

FREQUENCY : 100 kHz

Lab *j* →

Lab *i* ↓


	$D_i$ / (μV/V)	$U_i$ / (μV/V)
LNE	-10.3	15.3
AREPA	-5.8	25.6
NPL	-0.8	19.4
SP	11.2	18.5
IEN	-11.1	42.2
CEM	6.2	28.4
PTB	-1.5	21.4
NMi-VSL	-	-
INTI	-0.9	23.5
NMIA	7.1	17.3
NRC	4.1	22.1
VNIIM	-0.6	40.2
METAS	0.1	23.5
NIST	1.9	9.6
NIM	-5.5	12.3

OMH		JV		UME		CMI	
$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)	$D_{ij}$ / (μV/V)	$U_{ij}$ / (μV/V)
-	-	-22.1	39.6	-11.4	47.0	-7.4	62.2
-	-	-17.6	44.6	-6.9	51.3	-2.9	65.5
-	-	-12.6	41.4	-1.9	48.5	2.1	63.3
-	-	-0.6	40.9	10.1	48.1	14.1	63.0
-	-	-22.9	55.8	-12.2	61.3	-8.2	73.6
-	-	-5.6	46.3	5.1	52.8	9.1	66.6
-	-	-13.3	42.3	-2.6	49.3	1.4	64.0
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-
-	-	-11.7	43.5	-1.0	50.3	3.0	64.7
-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-

BEV	8.2	21.8
MIKES	5.9	10.0
INETI	11.2	30.6
OMH	-	-
JV	11.8	36.5
UME	1.1	44.4
CMI	-2.9	60.2

-	-	-3.6	41.9	7.1	48.9	11.1	63.7
-	-	-5.9	37.1	4.8	45.0	8.8	60.6
-	-	-0.6	47.1	10.1	53.4	14.1	67.2
-	-	-	-	-	-	-	-
-	-	-	-	10.7	57.0	14.7	70.1
-	-	-10.7	57.0	-	-	4.0	74.5
-	-	-14.7	70.1	-4.0	74.5	-	-

**CCEM-K9 and EUROMET.EM-K9 AC-DC transfer difference: 200 V, 100 kHz**  
**Degrees of equivalence,  $D_i$  and expanded uncertainty  $U_i$  (95 % level of confidence)**

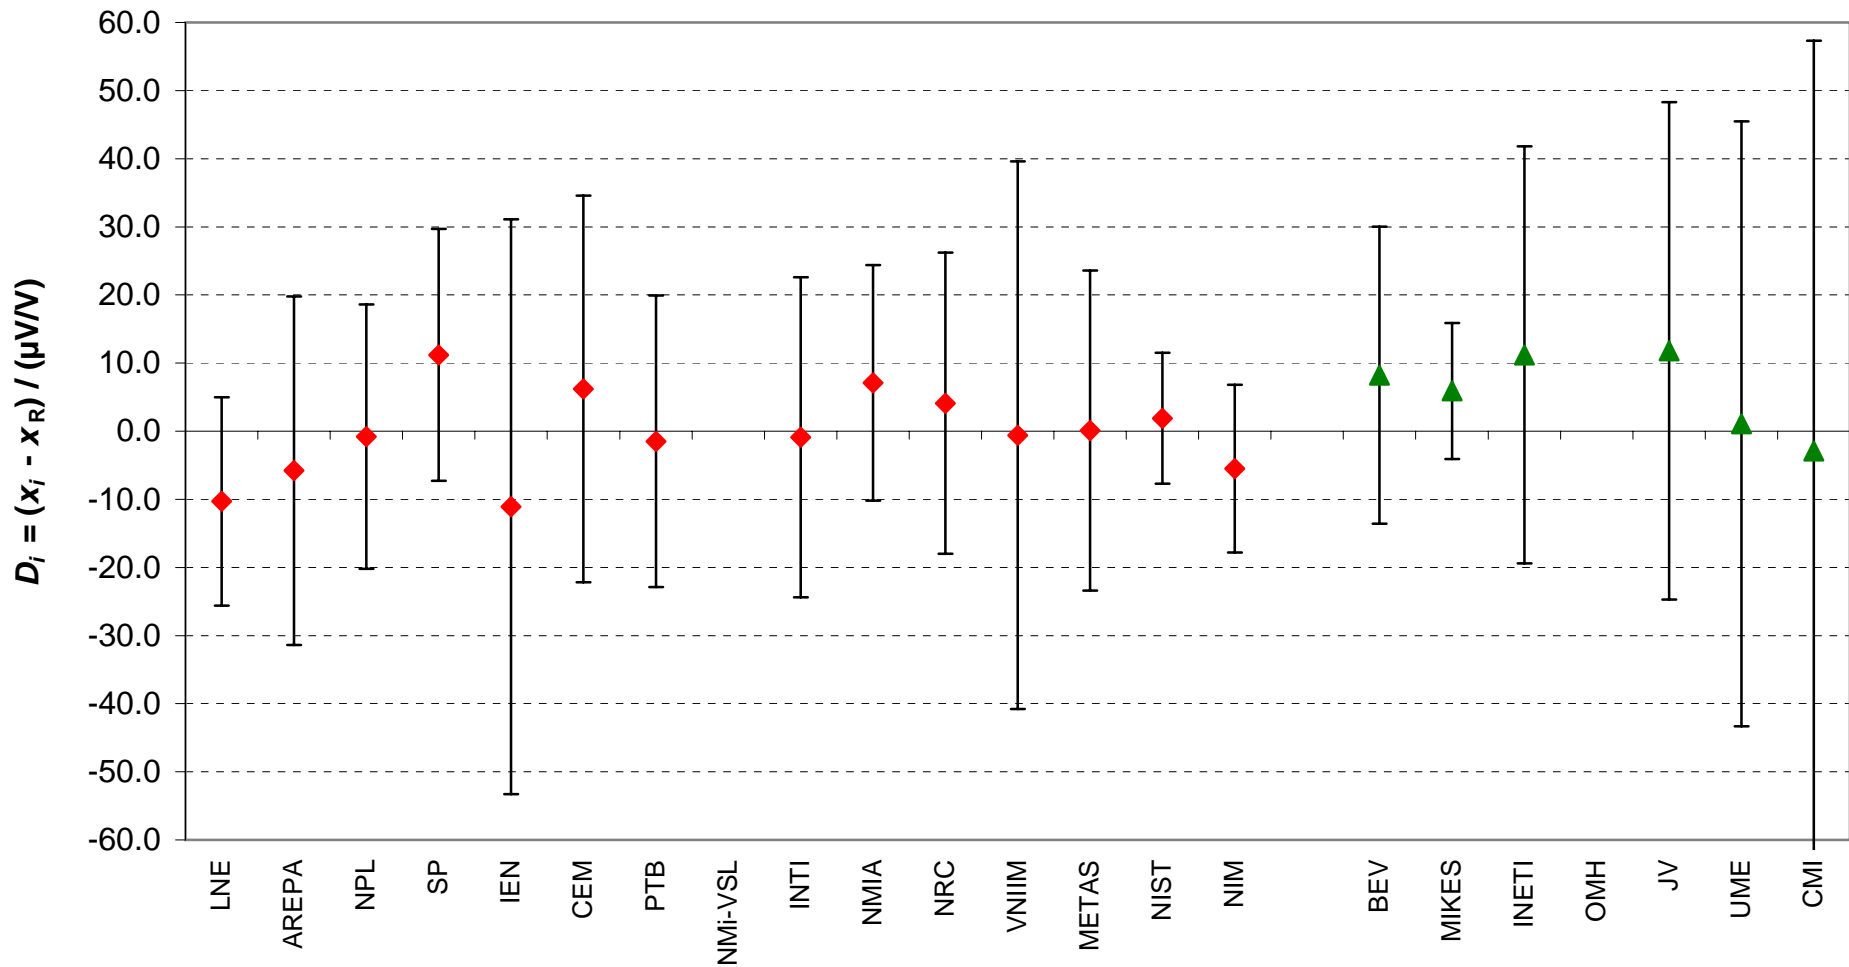

**Red diamonds:** participants in CCEM-K9, **Green triangles:** participants in EUROMET.EM-K9 only